PECCAT Computed Tomography Imaging X-ray System





175 Titus Ave, Suite 300 Warrington, PA 18976 Ph: 267-483-8081 Fax: 267-483-8086 info@curvebeam.com www.curvebeam.com CurveBeam Technical Support: 267-483-8081

pedCAT Table of Contents

Chapter	Name	Page
Chapter 1:	Introduction	3
Chapter 2:	Product Information	11
Chapter 3:	Safety Items	25
Chapter 4:	Calibration & Quality Assurance Procedures	37
Chapter 5:	Radiation Environmental Survey	56
Chapter 6:	Operations: Acquiring a Scan	71
Chapter 7:	Using the Viewing Software: CubeVue	93
Appendix I:	Installation Instructions	149
Appendix II:	Troubleshooting	161
Appendix III:	Scan Protocol Technical Details	171
Appendix IV:	Advanced Calibrations	173



CHAPTER 1: Introduction

In order to maintain the safety of patient's and operators of this device, it is important to operate and maintain the system correctly, following all instructions, warnings, cautions in this manual and labeling on the system itself. Installation Instructions are detailed in Appendix I.

The PedCAT has been evaluated against European MDD requirements and carries the C ϵ_{0413} mark.

For technical support or questions contact CurveBeam at 267-483-8081

Warnings, Cautions, Advice, and Notes:

Before attempting to operate the equipment, it is recommended that you read this manual thoroughly including all cautions and warnings. This guide uses the following conventions to describe situations that are potential hazards to the Patient or Operator, potential loss of data, or potential damage to the equipment.

Warnings are intended to alert the user that failure to follow the procedure could cause fatal or serious injury to the user, Patient, or any other person, or result in a misdiagnosis.

Cautions are intended to alert the user that failure to follow the procedure could cause damage to the equipment or cause loss of data.

Notes are used to highlight important or unusual points to be brought to the attention of the operator.

Advice Refer to user manual.

Safety Precautions:

WARNING The X-ray device is intended to be used for patients 50 lbs (23 kg) to 400 lbs (181 kg) and groin area at least 22" (56 cm) above the floor. DO NOT use this device for any patient less than 50 lbs (23 kg) OR groin area less than 22" (56 cm) above the floor, whichever is more restrictive.

WARNING The patient must wear a protective full wrap X-ray shielding apron (lead apron) during a scan. Patients less than 21 years old, small size patients (under 100 pounds) and children must also wear a gonad and ovarian front and back protective shield.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure.

WARNING Do not remove covers or cables on system. High voltage is present in the system. To avoid personal injury from electrical shock, do not operate the system with any covers open or cables removed.

WARNING This device may cause detrimental interaction with active implantable medical devices and body worn active medical devices. Consult the manufacturer of such devices for more information.

WARNING Closing of the Gate doors creates a pinch point. Keep hands and feet clear when closing Gate.

WARNING No modification of this equipment is allowed.

WARNING Service and maintenance can only be performed by CurveBeam authorized service personnel. ONLY Curvebeam authorized replacement parts can be used in the equipment. These requirements must be followed in order to avoid a hazard to the equipment, operator and/or patient.

CAUTION When initiating an exposure, the external Warning Light is activated a few seconds before the X-ray ON alarm (buzzer) and X-ray ON lights are activated.

CAUTION: Federal law restricts this device to sale by or on the order of a physician.

CAUTION: No auxiliary software should be installed on the system server and thin client terminals.

Electrical Hazards:

Installation and system wiring must meet all requirements of local governing authorities. Please check your local authorities and local codes to determine best practices for a safe installation. Do not place any liquid or food on any part of the consoles or other modules of the system. Observe all fire regulations. Fire extinguishers should be provided for both electrical and non-electrical fires. All operators should be fully trained in the use of fire extinguishers and other fire-fighting equipment and in local fire procedures.

WARNING In the event of an electrical fire, only use extinguishers that are labelled for that purpose. Using water or other liquids on an electrical fire can lead to fatal or other serious personal injury.

WARNING In the event of an electrical fire, to reduce the risk of electrical shock, try to isolate the equipment from the electric source before attempting to extinguish the fire.

WARNING To avoid risk of electric shock, this equipment must only be connected to a supply main with protective earth.

Explosion Hazard

Do not use the System in the presence of explosive gases or vapors, including anaesthetic gases. Use of this system in an environment for which it is not designed can lead to fire or explosion.

WARNING This unit is not suitable for use in a flammable air mixture environment. If hazardous substances are detected while the system is turned on, do not attempt to turn off the system. Evacuate the area and then remove the hazards before turning off the system.

Mechanical Hazards:

WARNING Do not operate the system with any covers open or removed. Operating the system with open or removed covers could expose mechanical operating systems that could cause serious or fatal personal injury to you or the Patient. Only qualified and authorized service personnel should remove covers from the system.

The system is designed to detect that the Gate doors are closed before a scan can initiate. If the gate doors are not closed, then the gantry will not engage and the x-ray will not initiate.

Laser Beam Hazards:

WARNING Laser beams can cause optical damage. The operator should avoid looking directly into the beams. The operator should instruct the patient to avoid looking directly into the beams. The use of optical instruments such as eyeglasses with large diopter or mirrors, increase eye hazard with this product.

Radiation Safety:

X-rays are dangerous to both operator and others in the vicinity unless established safe exposure procedures are strictly observed. Use the following safety measures to ensure safety to the Patient and Operator. The useful and scattered beams can produce serious or fatal bodily injuries to Patients and persons in the surrounding area if used by an unskilled operator. Adequate precautions must always be taken to avoid or reduce exposure to the useful beam or to scattered radiation. Operators are strongly urged to comply with the current recommendations of the International Commission on Radiological Protection and, in the United States, the US National Council for Radiological Protection.

Use the following measures to protect yourself and the patient from unintended exposure to radiation. Anyone who is near the patient during test procedures must observe the following precautions:

- Maintain distance from exposed radiation source in accordance with the facility survey or site plan and shielding designs, provided by a medical physicist. The plan/survey will be created based off of Scatter Measurements provided in this manual. Refer to "typical pedCAT Layout" towards the end of Chapter 5 of this manual for additional details.
- Keep exposure times to a minimum.
- Patient must wear protective X-ray shielding items (lead apron, etc.) to protect anatomical areas. We recommend all patients wear a protective shielding full wrap apron. We recommend that patients less than 21 years old, small size patients (under 100 pounds) and children also wear a gonad and ovarian front and back protective shield. Sample shielding products, or similar: Supplier: Marshield, Full Wrap Apron, #MS-SP1 Supplier: Universal Medical Inc, Diaper 14" x 20", #800
- Wear a PEN dosimeter and/or film badge.
- If you are required in the exam room during a procedure, stay as far from the scanner as possible or behind a mobile protective wall.
- The physician is responsible for protecting the patient from unnecessary radiation.

System Safety Devices:

They system safety devices include an Emergency Stop, Warning System, and Interlock System. These are explained fully in Chapter 3 – Safety Items.

Patient Preparation Recommendations:

We recommend the patient wear FDA approved medical gloves for gripping the hand rails, with sanitation and convenience in mind.

We also recommend the patient not step bare foot on the patient platform. Proper foot protection should be provided.


After each patient scan, clean and disinfect all items which come in contact with the patient.

Cabling Requirements:

System cabling connections must be installed away from walkways and doorways. It is recommended to run cabling along wall perimeters. If there is a chance of mechanical damage due to the cable location, then the use of conduit or other means of protection should be considered.

System Description

The PedCAT is a Computed Tomography X-ray system or Cone Beam Volumetric Tomography x-ray system for 3D reconstruction Imaging device for the foot and ankle. The system is designed for an in-office setting with components consisting of the Scanner, Operating Computer (External Server), Operator's Console and Viewing Console. The system provides for patient's to be imaged in weight bearing (standing) position as well as seated position for one or both feet.

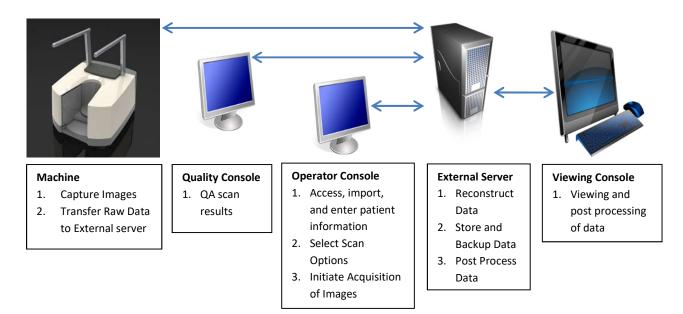

The External Server consists of 4 Virtual Machines:


ACQ VM: accessed via the Main Desktop icon on the ACQ thin client terminal

Viewing Station/MD VM: accessed via the Main Desktop icon on the QCW thin client terminal or the QA Station thin client terminal.

RECON VM: accessed via Remote Desktop Connection icon on the ACQ thin client terminal.

Database VM: accessed via Remote Desktop Connection icon on the ACQ thin client terminal.

Major Device Components:

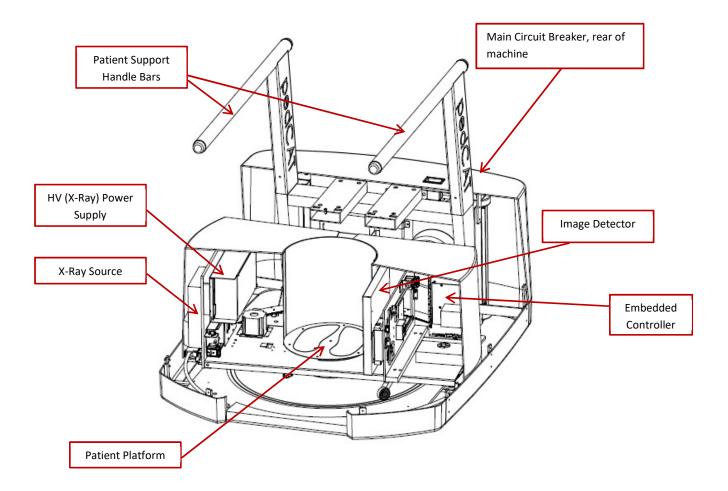

Intended Use of the Device:

The PedCAT is intended to be used for 3-D imaging of the foot & ankle region, to visualize and assess the osseous and certain soft tissue structures, including joint spaces, bone angles and fractures. This modality is anticipated to be applicable to pediatric* cases as well as adults*, when appropriate diagnosis of a given foot condition is considered necessary.

* Patient parameters: 50 lbs to 400 lbs Groin area at least 22" above the floor

8

Major System Items:

- Scanner
- Dell server with hard drives, network cards, DVD drive, etc and Uninterrupted Power Supply (UPS)
- External Cable Kit
 - Door Interlock, 50' (15.24 m)
 - Warning System, 50' (15.24 m)
 - Door interlock, shorting plug
 - Operator Control Box Assembly, 50' (15.24 m)
- Ethernet Cable, CAT6, gray, 50' (15.24 m) (QTY 2)
- Ethernet cable, CAT 6, green, 50' (15.24 m)
- Ethernet cable, CAT6, red, 50' (15.24 m)
- Power cord, 10' (3.05 m)
- Varian Panel, 3030D
- X-Ray tube assembly
- X-Ray power supply

Intended User Profile:

The PedCAT is intended to be used by an operator that meets all local, state, federal or international regulations and that has been trained by CurveBeam personnel using the PedCAT On Site Training Checklist.

About the Operators' Manual:

This documentation describes the safe and effective operation of the system. The information is intended to provide trained Technologists and Physicians the necessary guidance to operate the system in a safe and effective manner.

CurveBeam assumes no liability for the use of this document if any unauthorized changes to the content or format have been made.

Conventions Used in the User Manual:

Main Menu items and Tabs are in quotes (" "). Software Programs are in quotes (" ")

Interface buttons are capitalized" (BUTTON).

Standard Limited Warranty

CurveBeam, LLC warrants the original purchaser that this hardware system will be free from defects for a period of one (1) year from the date of delivery. During the warranty period, CurveBeam, LLC will correct any defects in material or workmanship, at no charge for material, labor or travel. Any replacement parts shall be new or serviceable used parts and are warranted for the remainder of the original warranty or thirty (30) days, whichever is longer. This original warranty includes software maintenance upgrades^{*}, but excludes new optional application modules or major new features. Also included in the warranty is free telephone consultation which will be furnished without charge by CurveBeam LLC. Data back-up is not covered and is the customer's responsibility.

* CurveBeam, LLC reserves the right to determine which software upgrades are included in the warranty.

The warranty period is not extended as a result of purchasing any additional parts from CurveBeam, LLC. The original purchaser must promptly notify CurveBeam, LLC in writing if there is a defect in material or workmanship. Written notice in all events must be received by CurveBeam, LLC before expiration of the warranty period. This warranty is not transferable. This One-Year Limited Warranty covers normal use.

CurveBeam, LLC does not warrant or cover the following:

- Damage caused by impact with other objects, dropping, falls, spilled liquids or immersion in liquids
- Damage caused by a disaster such as fire, flood, wind, earthquake, or lightning
- Damage caused by unauthorized attachments, alterations, modifications or foreign objects
- Damage caused by failure to provide a suitable operating environment
- Damage caused by the use of the hardware system for purposes other than those for which it was designed
- Damage from improper maintenance performed by other than OEM trained personnel
- Damage from improper electrical connection or supply
- Damage caused by any other abuse, misuse, mishandling, or misapplication
- Damage to internal or external computer, software, or operating system caused by:
 - \circ $\,$ Unauthorized additions or changes, Viruses, spyware or gaming software
 - Applications other than its intended use
 - Damage caused by third party software or damage caused by unauthorized changes to the system software
 - Damage caused by unauthorized upgrades, additions, deletions or unnecessary internet use, or any other unauthorized application.
- Under no circumstances shall CurveBeam, LLC be liable for any special, incidental, or consequential damages based upon breach of warranty, breach of contract, negligence, strict liability or any other legal theory. Such damages include, but are not limited to, loss of data, loss of profits, loss of revenue, loss of use of hardware system or any associated equipment, cost of capital, cost of substitute or replacement equipment, facilities or services, down time, purchaser's time, the claims of third party, including customers, and injury to property.

Disclaimer of Warranties The warranty stated above is the only warranty applicable to this product, all other warranties, expressed or implied including all implied warranties of merchantability or fitness for a particular purpose, are hereby dis-claimed. No oral or written information or advice given by CurveBeam, LLC, its agents or employees shall create a warranty or in any way increase the scope of this warranty.

CHAPTER 2: Product Information

Technical Specifications:

Description	Specification
Tube voltage	100 kVp, 120 kVp, (+/-10%)
Tube current	5 mA, (+/-10%)
CBCT Scan time*	16-32 sec
CBCT Procedure time**	Medium Field (MFOV): 50 sec,
	Large Field (LFOV): 106 sec
Max exposure time (based on typical pulse width)	10 sec
Image detector	Amorphous Silicon flat panel
Gray scale	14 bit
CBCT Imaging Volume	7.9" (20 cm) high x 13.8" (35 cm) diameter,
	7.9" (20 cm) high x 7.9" (20 cm) diameter
Typical slice thickness	0.5mm (+/-0.5mm); Slice Spacing 0.30 for MFOV, Slice
	Spacing 0.37 for LFOV
Typical voxel size	0.3 mm voxel for MFOV, 0.37 mm voxel for LFOV
Measurement accuracy	± 2 voxel
Body part scanned	Foot and ankle
Size of system: h x d x w	47"x59"x48" (119.4 cm x 149.9 cm x 121.9 cm)
Weight	400 lbs (181.8 kg)
Power Requirements	1150VA

*Scan time is defined as the duration in which the exposure alarm (buzzer) is ON and X-ray ON light is illuminated.

**Procedure time is from time the exposure button is pressed to when the doors open completely after the scan.

X-ray Source:

Tube Voltage:	100 kVp(eff), 120 kVp(eff), +/- 10%
Tube Current:	5 mA, +/- 10%
Voltage Wave Shape:	Constant Potential
Focal Spot:	0.0197 inches (0.5 mm)
Duty Cycle:	3%
Source to Sensor distance:	28.896" (73.39 cm)
Source to Patient distance:	21.095" (53.58 cm*)

*The patient must be properly positioned for each patient for all applications in order to have the focal spot to skin distance as large as possible.

Minimum Filtration (at 120 kVp(eff)) (mm of aluminum equivalent): 10 mm or greater

Maximum Rated Continuous Tube Operation: 130 kVp @ 0.5 mA

Maximum Rated Pulsed Tube Operation: 130 kVp @ 5mA

NOTE: Leakage technique factors are measured at the maximum specified energy.

Timer: ± 0.1 seconds or 5%, whichever is greater

X-ray Beam Size: 2 Rectangular: 11.8" (30 cm) wide x 11.8" (30 cm) high, 5.9" (15 cm) wide x 5.9" (15 cm) high

Image Detector: Amorphous Silicon Flat Panel (readable area): 11.8" (30 cm) height x 11.8" (30 cm) width.

Sensor Front Panel Attenuation Value: Less than 1mm of aluminum equivalent (information for reference only)

Gray Scale: 14 bit

Voxel Size: 0.3 MFOV / 0.37 LFOV

CBCT Image Acquisition: 1 or 2 orbits, 360 degree rotation (maximum)

CBCT Field of View: 7.9" (20 cm) diameter x 7.9" (20 cm) height (1/2 or 1 orbit)


CBCT Extended Field of View: (offset scan): 13.8" (35 cm) diameter x 7.9" (20 cm) height (2 orbits)

CBCT Procedure Times: 50 sec for 20 x 20, 104 sec for 35 x 20

Patient Protocol options available for scanning:

Patient Parameters	Exposure Factors	Туре
Small Size: Weight: 50 to 100 lbs (23-45 kg), Height: Groin area at least 22" (56 cm) above the floor.	100 kVp, 5mA	Small Patient: Medium Field (100kVp)
<i>Small Size:</i> Weight: 50 to 100 lbs (23-45kg), Height: Groin area at least 22" (56 cm) above the floor.	100 kVp, 5mA	Small Patient: Large Field (100kVp)
Weight: 101 to 400 lbs (46-181 kg), Height: Groin area at least 22" (56 cm) above the floor.	120 kVp, 5mA	Large Field (120kVp)
Weight: 101 to 400 lbs (46-181 kg), Height: Groin area at least 22" (56 cm) above the floor.	120 kVp, 5mA	Medium Field (120kVp)
Weight: 101 to 400 lbs (46-181 kg), Height: Groin area at least 22" (56 cm) above the floor.	120 kVp, 5mA	Medium Field, Sharp Filter (120kVp)

Minimum patient size parameters:

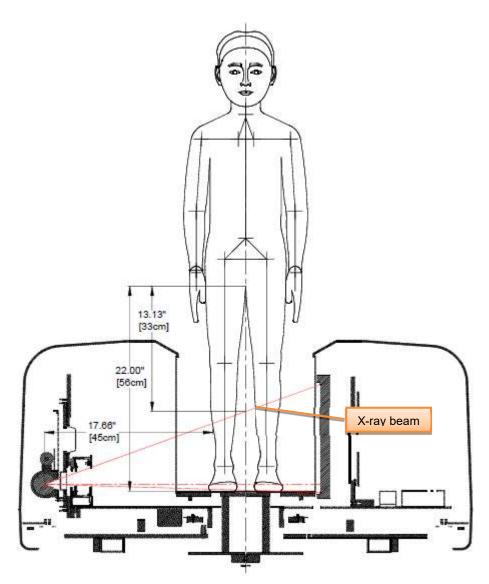

CBCT Primary Reconstruction:

- Medium Field of View options: Maximum 2 minutes
- Large Field of View options: Maximum 3 minutes

CBCT Secondary Reconstruction: Real Time

Gantry Stopping Distance and Angle: Total rotation from Home position to limit is 424 degrees (Home being 0 degrees). "Load" position (gantry aligned for patient to walk in) is 25 degrees from home position.

Power Requirements:

The Scanner requires a Dedicated Line and/or Filtered Line. A Surge Protector is recommended. The Scanner is suitable for continuous connection to a power supply in stand-by mode.

Line Voltage: 100VAC, 115VAC, 200VAC all ± 10% (Factory Set)

210 to 240VAC (which covers 220, 230 and 240 VAC power supplies) (Factory Set)

Line Current: 10 Amps (100V), 10 Amps (115V), 5 Amps (200V) or 5 Amps (230V)

Line Frequency: 50 Hz / 60 Hz

Phase: Single

Main Circuit Breaker: 10 Amps (100V), 10 Amps (115V), 5 Amps (200V), or 5 Amps (230V)

Nominal Electrical Input Power to Supply: Volume Scan = 300W (120kV, 5mA); Scan Time has no effect on electrical power output.

Apparent Resistance of Supply Mains:

For the purpose of obtaining the apparent resistance of supply mains, resistance is determined according to the following formula:

R= <u>UO – U1</u> <u>I1</u> Where: U0 is the no-load Mains Voltage U1 is the Mains Voltage under load. I1 is the Mains Current under load.

Circuit Breaker Assembly	UO	UI	11	Apparent Resistance
100VAC	100VAC	98.8VAC	2.5A	0.48ohms
115VAC	115.4VAC	114.2VAC	2.1A	0.57ohms
200VAC	200.4VAC	198.1VAC	1.3A	1.77ohms
230VAC	230.8VAC	228.0VAC	1.2A	2.33ohms

Environmental Specifications:

Operating:

- The operational temperature range shall be 59°F to 86°F (+15°C to +30°C).
- The operational humidity range shall be 25 to 60% relative humidity, noncondensing.
- The minimum time period that the room environmental operating conditions must be maintained prior to powering the system is 1 hour.

Transportation and Storage:

- The storage and transport temperature range shall be -4°F to 122°F (-20°C to +50°C).
- The storage & transport humidity range shall be 10% to 95% relative humidity, noncondensing.

Scanner and Acquisition Computer (server):

• Requires a Dedicated Line and a Surge Protector is recommended.

Patient Platform:

• Maximum patient weight capacity: 400 lbs. (181kg)

Patient Seat:

• Maximum patient weight capacity: 300 lbs. (136kg)

Handle Bars:

• Maximum weight capacity: 150 lbs. (68kg)

Disposal:

Follow local regulations on disposal of waste parts. The *X-ray source assembly, image sensor* and *all electronic circuits* should be regarded as non environmental friendly waste product. The system does not generate, or require the use of, any materials that require special disposal instructions as part of regular operation.

Extension Cords:

Do not use any extension cords which are not provided with the system. Be aware that multiple portable socket outlets or extension cords are not to be connected to the system.

External Items:

Do not connect any items or equipment to this system which are not part of the system.

Electromagnetic or other Interference (Emissions and Immunity):

The system was tested and it was determined to meet the class A (non-residential) limits. The system pass testing with a reduced level of compliance with the criteria contained in IEC 60601-1-2 Edition 3 Issued 03/2007.

Test Name	Test Level/ Equipment Class	Results/Notes	Immunity Performance Criteria Met
	Emissions Testin	Ig	
Radiated Emissions	Class A: Group 1	Compliant	-
Conducted Voltage Emissions	Class A: Group 1	Compliant	-
IEC61000-3-2 Harmonic Current Emissions	Class A	Compliant	-
IEC61000-3-3 Voltage Changes, Voltage Fluctuations and Flicker	Class A	Compliant	-
	Immunity Testing	g	
61000-4-2 Electrostatic Discharge	±6 kV Contact, ±8 kV Air	Compliant	A
61000-4-3 Radiated Immunity	80 MHz – 2.5 GHZ, 3 V/M, 80% AM with 1kHz	Compliant	A
61000-4-4 Electrical Fast Transients	±1 kV Power Supply Lines, ±1 kV Input/Output Lines	Reduced Level of Compliance	A
61000-4-5 Surge Immunity	±1 kV Line to Line, ±2 kV Line to Earth	Compliant	A
61000-4-6 Conducted Immunity	150 kHz – 80MHz, 3 Vrms	Compliant	A
61000-4-8 Power Frequency Magnetic Field	3 A/M	Compliant	A
61000-4-11 Voltage Dips and Short Interruptions	>95% dip for 0.5 periods	Compliant	A
	60% dip for 5 periods	Compliant	A
	30% dip for 25 periods	Compliant	A
	>95% dip for 5 seconds	Compliant	С

WARNING This system is intended for use by healthcare professionals only. This system may cause radio interference or may disrupt the operation of nearby equipment. Follow the following recommendations below.

Recommended separation distances between portable and mobile RF communications equipment and the PedCAT

The PedCAT is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the PedCAT can help prevent electromagnetic interference by maintaining a minimum distance of 10 feet (3 m) between portable and mobile RF communications equipment (transmitters) and the PedCAT. Refer to the portable and mobile RF communications equipment user's manual for recommended clearance distances to other equipment based on the maximum output power of the communications equipment. Maintain a minimum distance of 10 feet (3m) between the PedCAT and portable and mobile RF communication equipment.

Equipment Standards:

The PedCAT has been designed and evaluated to meet the requirements of the following standards. The device has passed all applicable sections of these standards.

IEC 60601-1, third edition, 12/2005 IEC 60601-1-2, third edition, 03/2007 IEC 60601-1-3, second edition, 01/2008 IEC 60601-1-6, third edition, 01/2010 IEC 60601-2-7, second edition, 02/1998 IEC 60601-2-44, third edition, 02/2009 IEC 62304, first edition, 05/2006 ISO 15223-1:2012 ANSI/AAMI ES60601-1, third edition, 01/2005 CSA C22.2 NO. 60601-1:08-CAN/CSA, third edition, 07/2008 BS EN ISO 14971:2009 EN ISO 15223-1:2012 BS EN 1041:2008

IEC 60601-1, second edition, 12/1995

IEC 60601-1-3, first edition, 01/1994 IEC 60601-1-6, first edition, 01/2006 IEC 60601-1-8, first edition, 1/2003

IEC 60601-2-44, second edition, 01/2002

The PedCAT conforms to the provisions of MDD 93/42/EEC (as transposed into national law in the United Kingdom through Statutory instrument SI 618 2002 Medical Device Regulations 2002 and as amended by SI 2008 No. 2936).and Australian Medical Device Directives, TGA, v1.1, May, 2011

Equipment Class:

- Protection against electric shock: Class I
- Applied part has degree of protection against electric shock: Class B
- Class of equipment against ingress of liquids: Ordinary Equipment: IPX0
- Radiated emissions: Class B

Regulatory Class:

Governing Body	Classification
FDA	2
Health Canada	3
Medical Device Directive(93/42/EEC)	llb

Cleaning:

Routinely and after each patient scan, clean and disinfect all items which come in contact with the patient.

Cleaning the equipment frequently, especially if corroding chemicals are present is a function of the Operator. Unless otherwise instructed, use a cloth **moistened** with warm water and mild soap. Do not use strong cleaners and solvents as these may damage the finish. <u>Be careful when cleaning to avoid liquid leaking underneath the Platform Area and into the Gantry</u>. DO NOT USE WATER ON THE IMAGE RECEPTOR, this should only be dusted with a dry cloth.

For disinfecting, use Biocide ® from Biotrol International or equivalent cleaner and disinfectant. Biocide® is an Iodophor formulation that kills HIV, Tuberculosis and Polio in 10 minutes. Moisten a cloth with the disinfectant and then wipe down the area. Do not spray disinfectant directly onto the equipment.

Preventive Maintenance Schedule - for Owner / User:

• Daily:

Routine Dusting - all surfaces.

Clean and Disinfect all items which come in contact with the patient after each patient scan.

• Monthly:

Clean/Disinfect all surfaces, check for failed/faulty indicator lights.

• Quarterly:

Perform Panel Calibration (Gain, Air)

• Yearly:

Check for satisfactory image quality.

IT IS THE RESPONSIBILITY OF THE USER TO INSURE THAT THE EQUIPMENT IS MAINTAINED IN COMPLIANCE WITH THE MANUFACTURER'S RECOMMENDED MAINTENANCE SCHEDULE. THE MANUFACTURER AND THE ASSEMBLER / INSTALLER ARE RELIEVED FROM RESPONSIBILITY IN THOSE CASES WHERE NON-COMPLIANCE WITH THE STANDARD RESULTS FROM THE USER'S FAILURE TO HAVE THE MANUFACTURER'S RECOMMENDED MAINTENANCE PERFORMED.

The actual maintenance inspection and consequent service must be accomplished either by an authorized factory trained technician or by a competent serviceman of the user's choice who has adequate training in those aspects of the Performance Standards of the Radiation Control for Health and Safety Act of 1968 that are applicable to this equipment. Neither the inspection nor service is part of the equipment warranty. (To be arranged for by the Owner or User with the Dealer's Service Department).

Planned Maintenance – Monthly Schedule:

The system requires monthly maintenance check for failed or faulty indicators/lights.

 Procedure for checking for failed or faulty indicators/lights. If any of the below do not behave as expected, then please contact CurveBeam Technical Support at the number on the front cover of this manual. CB-ToolShed Program:



- From the ACQ Desktop area, click on the CB-ToolShed icon. This icon will open the interface required for the checks.
- WARNING LIGHT: In this interface, first click on WARNING LIGHT TEST button. If your system has a warning light installed, then the WARNING LIGHT should turn ON. If the warning light does not function check the electrical connections, power and indicator lights/audible alarms for proper operation. If the warning system components are found functional then contact CurveBeam Technical Support.
- DOOR INTERLOCK: Next, if you have a Door Interlock, first close the X-ray Room Door. Click on the DOOR INTERLOCK TEST button. If functioning

properly, then a message will appear indicating so. Then Open the X-Ray Room Door and click on the DOOR INTERLOCK TEST button again. The message should indicate that the Door is opened and no x-ray can be taken at this time.

- EXPOSURE: This will check the Exposure Switch, audible exposure sound and both visual X-Ray ON indicator lights. Click on the EXPOSURE TEST button. An instruction should display asking to "Push and hold down the exposure button". Hold down the exposure switch for the duration of the exposure, which should be approx. 5 seconds. Observe for the audible sound and that the X-ray ON lights on the machine and the operator's control box are illuminated in Amber color during this exposure.
- EMERGENCY STOP: Exit the CB-Tools program by clicking on the X in the upper right corner. With the machine Main Circuit Breaker in the ON position, Power Light ON, press the EMERGENCY STOP button. The Main Circuit Breaker should trip. Release the EMERGENCY STOP by turning the knob to the right until it pops up. Turn the Main Circuit Breaker to the ON position and relaunch the PedCAT ACQ Software.

Planned Maintenance – Quarterly Schedule:


The system requires quarterly maintenance check for Panel Calibration. This can be performed by the end user with CurveBeam Technical Support if necessary.

 The procedure for the panel calibration is in the section under <u>Calibration</u> <u>Procedures</u>.

Advice: Please refer to that section for instructions on performing this procedure. (Chapter 4: Calibration and Quality Assurance Procedures).

If panel calibrations are not routinely performed, there may be suboptimal image quality. The scan results may have symptoms of artifacts commonly referred to as "circle or ring artifacts". Below are samples of circle artifacts in scan results. If these are observed than a panel calibration should be performed.

Advice: Please refer to Chapter 4 and also contact CurveBeam Technical Support.

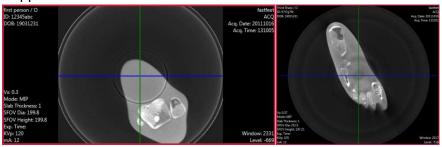

UPS (Uninteruptible Power Supply) Maintenance:

Please refer to the Tripp Lite UPS (SMART1500LCDT 120v 1500va 900w and SMX1500LCDT 230V 1.5kVA 900W) User's Guide for UPS maintenance recommendations.

Planned Maintenance - Annual Schedule:

The system requires normal periodic inspection and maintenance. Scheduled periodic inspections are necessary to detect problems which can result from excessive wear, loose items, chafing wires, and mis-adjusted parts from continual system use. In addition to mechanical inspection and calibration, a series of image performance tests are to be conducted. Planned maintenance is to be performed annually by a factory trained Service Technician. If there are any questions regarding the annual maintenance, please contact CurveBeam Technical Support.


Replacement Parts:


Part Description	Part Number
Gantry Belt	200104
Rotation Motor	100109
Beam Limiter Motor	100112
Receptor Motor	100110
Door Motor, left, programmed	2010-10
Door Motor, right, programmed	2011-10
Breaker Switch Assembly 100 VAC	4002-100-0
Breaker Switch Assembly 115VAC	4002-115-0
Breaker Switch Assembly 200VAC	4002-200-0
Breaker Switch Assembly 230VAC	4002-230-0
X-Ray Power Supply Assembly	4003-0
Embedded Board Assembly	4004-0
Can Bus Breakout Assembly	4006-0
120VAC Breakout Assembly	4007-0
LED Distribution Assembly	4008-0
X-Ray Tube head	2007-0
Image Receptor (Panel)	100100
Ethernet Cable CAT 6 GREEN, 50'	100105
Ethernet Cable CAT 6 RED, 50'	100106
Operator's Control Box	5006-0
Scan (Exposure) Switch	5007-0
Geometric Phantom	2803
QA Phantom	2802

Accessories:

The system has no accessories.

System Dimensions:

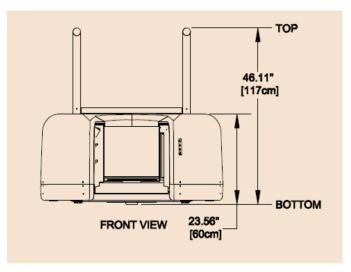



CHAPTER 3: Safety Items

In order to maintain the safety of patients and operators of this device, it is important to operate and maintain the system correctly, following all instructions, warnings, cautions in this manual and labeling on the system itself.


System Safety Devices:


Emergency Stop: In the event of an emergency (any moving component collides with any parts of the equipment or items in the environment, or that could cause physical injury to the Patient), the Operator or Patient should utilize one of the 2 designated Emergency Stop buttons to turn off the power to the X-ray and all moving parts in order for the Patient to be safely removed from the machine. There is an Operator E-stop button on the Operator Control Box and there is a Patient E-Stop button on the machine by the seat. The Emergency Stop (s) when activated will remove ALL power from the machine. If the machine gates are closed, they will have to be opened manually and any obstructions to the patient exit manually removed.

Warning System: The System is equipped with provisions for warning lights and/or audible alarms when X-ray power is energized. An externally powered Warning System can be connected to the cable provided which is capable of 250 volts, 50/60 hertz, and 1 amp. When X-ray power is energized the warning system is also energized.

Interlock System: This System is equipped with provisions for an Interlock Circuit which, when opened, will turn off X-ray power. This is a low voltage circuit, 5 volts DC. To use the Interlock Circuit disconnect the factory installed Shorting Plug. Connect the supplied Interlock Cable to the scanner. Connect door switches (NO/COM terminals) and/or emergency stop switches (NC/COM terminals) in series between the other end of the Interlock Cable wires. Multiple door switches and/or emergency stop switches can be connected as long as the devices are connected in series. The entire circuit must be a closed loop when all of the doors are closed and/or emergency stop switches are in their normally closed state.

Whenever the door switch or switches are opened or emergency stop button(s) pressed the X-ray power will be turned off. X-ray power cannot be turned on when the interlock circuit is open.

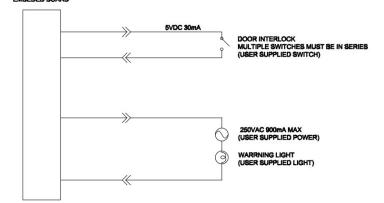



Patient Preparation Recommendations:

We recommend the patient wear FDA approved medical gloves for gripping the hand rails, with sanitation and convenience in mind.

We also recommend the patient not step bare foot on the patient platform. Proper foot protection should be provided.

After each patient scan, clean and disinfect all items which come in contact with the patient.

Cabling Requirements:

System cabling connections must be installed away from walkways and doorways. It is recommended to run cabling along wall perimeters. If there is a chance of mechanical damage due to the cable location, then the use of conduit or other means of protection should be considered.

Emergency Removal of a Patient:

The system has undergone extensive testing of the mechanically, electrically and software performance, but if an unexpected occurrence is observed and/or the software locks up during a scan or an emergency arises where it becomes necessary to interrupt a scan and/or remove a patient from the system before a scan is completed, please follow these steps:

1. Press the EMERGENCY STOP button. This will halt the X-ray as well as the motors to the machine functions and all power to the machine. The message below will display on screen and will terminate the "CB Scanning Device" Acquisition software:

C _{IB}	
MicroController Seq The application will Please restart the sys and if the behavior p contact technical su	pe terminated. tem, persists,
GoodBy	/e

2. Open the Gate doors manually with your hands by using the slots at the top of each door to grasp and slide to an open position.


3. Carefully assist the patient to step out of the scan platform area.

4. Reset the machine: Close the PedCAT Acquisition, "CB Scanning Device" software (if not already). Release the E-stop by turning the knob to the right until it pops up. Then turn the machine power back ON at the Main Circuit Breaker. Re-launch the PedCAT Acquisition "CB Scanning Device" software. Now the system can be operated again as expected.


In the case of loss of power to the scanner, perform Steps 1-3 above. Once power is restored, Step 4 can be performed.


System Labels:

Operator Control Box: E-Stop, Power ON light, X-ray Ready light, X-ray ON light, Fault light, Scan/Exposure Button.

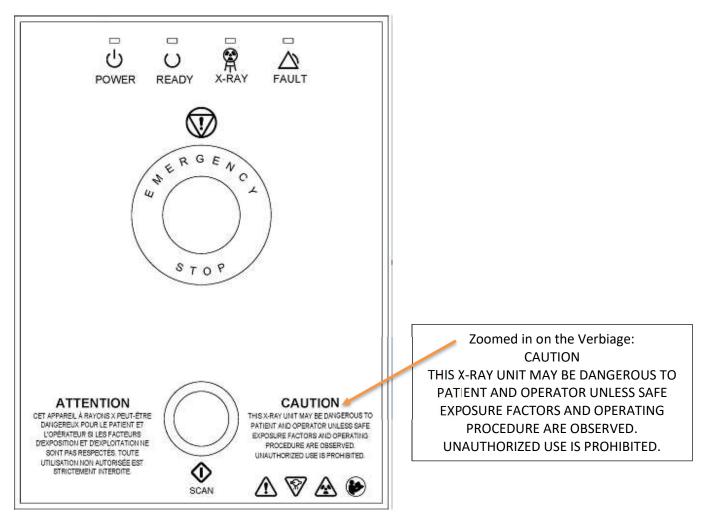


Rear Connector Panel:

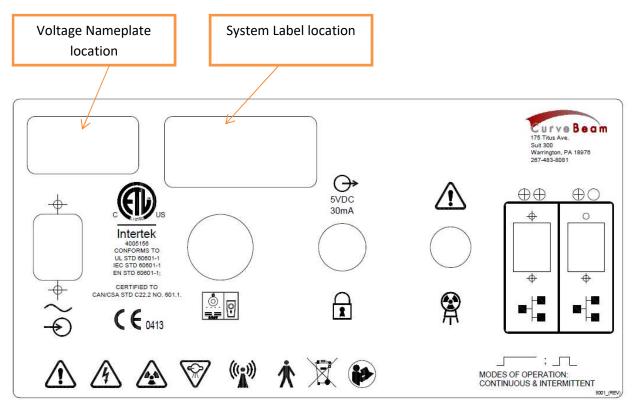

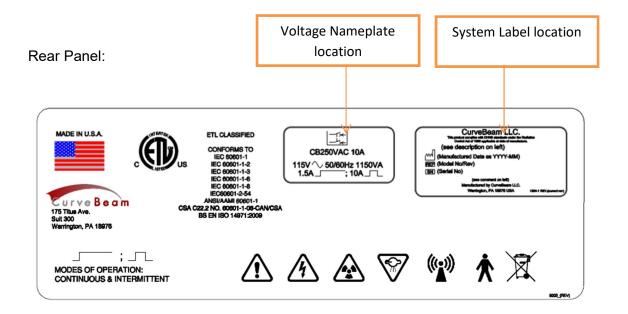

Voltage Nameplate for opening in Rear Connector Panel and Rear Panel:

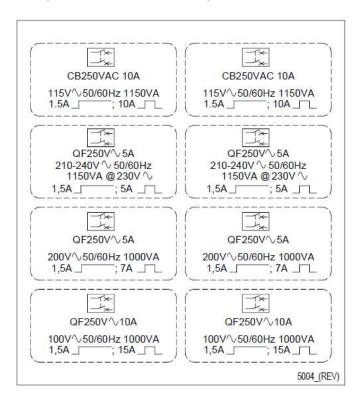


Indicator Panel (on machine):




Patient Platform label:



Patient Seat label:



Handle Bar Label:



Cleaning Instructions Label:



Pinch Point Label:




Laser Label:



Laser Switch Label:




Circuit Breaker and Fuse Label:

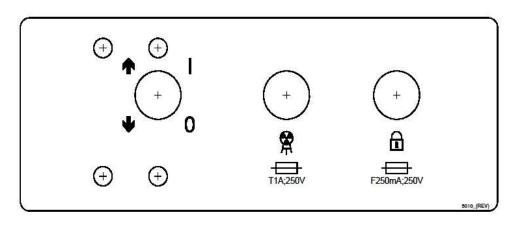

X-ray Protective clothing label (located on the handle bar):



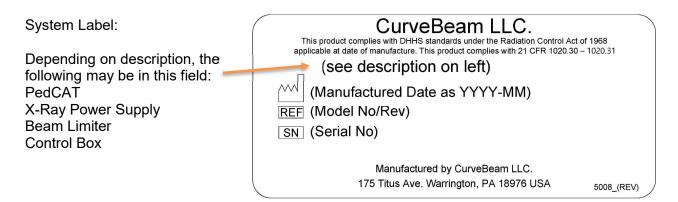

Tube Head Label:



Tubehead Focal Spot Label:



SYMBOL	SYMBOLS:							
	eneral /arning		lonizing Radiation		Electrical Haz	zard	$\sim \rightarrow$	AC In
	mergency top	\bigtriangledown	X-Ray Radiation	(((•)))	Non-Ionizing Radiation			Network Cable
U Po	ower		Follow Operating Instructions for use.	T	Type B (body) applied part con with IEC 60601-		. <u>©.</u>	Control Box
U R	Ready	\Diamond	Scan	X	Recycle			Pinch Point
×	-Ray On		Laser	⊖→ 5VDC 30mA	Output for Inte	rlock	ن م _ت	Maximum weight capacity for sitting.
	ault	n B	Maximum Weight capacity for standing.	T	Interlock		· /	Maximum weight capacity for handle bars.
F F	use	I Pov	wer/Circuit ON		CE Mark			
T1A250V, delay, 1amp fuse F250mA25 acting, 250n fuse	o, 250volt 50V, F=fast	0 Pov OF	wer/Circuit F	This product carries the CE Mark. The CE Declaration (CE Conformity) becomes invalid if the product is changed without explicit consent of the manufacturer! This applies to all not only to safety elements.		(CE Conformity) becomes ct is changed without explicit nufacturer! This applies to all parts,		
					class IIb			

European Authorized	CurveBeam Europe Limited	
Representative:	Devonshire House	
•	1 Devonshire Street	
	London W1W 5DR	

System Controls and Indicators:

Operator Control Box:

The Operator Control Box contains the status indicator lights as well as the Emergency Stop button and the Exposure Control Switch. This can sit on a table or be mounted on a wall. It is equipped with a 50 foot cable.

Operator Control Box Status Indicator Lights: For Power ON, Exposure Ready, O, X-RAY FAULT Exposure ON, Fault. Exposure Control: Scan Button for initiating the scan. Must be held down for the duration Emergency Stop Button of the capture. Press down if the exposure needs The duration of the exposure will to be stopped. This will seize be indicated by an audible signal exposure, and motors. The button generated by the workstation and will also illuminate. machine, as well as visual X-ray **ON** lights To Reset the button, turn it to the right so it pops out.


Patient Emergency Stop Button:

This Emergency stop button is intended for the patient to stop exposure during a scan. This will seize exposure and all motors. It is located on the machine itself, by the seat, as shown below. To Reset the button, turn it to the right so it pops out.



Patient Alignment Laser Lights:

There are 3 patient alignment laser lights on the machine. There is a horizontal and vertical in the center of the beam, and a horizontal at the top of the beam height. The patient alignment laser lights are controlled by a push button on the machine on the left door when open. When the button is pushed and held down, the lights will illuminate.

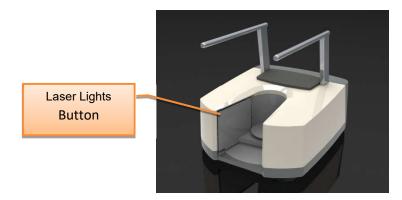

System Status Indicators

There are 4 indicator lights. These indicator lights are on the Operator's control box and on the machine itself on the upper right cover. There are also similar indicators within the Acquisition software program.

The lights are as follows:

- **POWER Power ON:** This is solid **Green** when the machine is ON.
- **Ready:** This is the Exposure Ready light and is **Green** when the machine is in Ready state for exposing. This would indicate that it is time to press the exposure button.
- X-Ray ON: This is an Amber color when the system is exposing, emitting X-ray.
- **FAULT** Fault: This would be **Red** in color if there was a failure in the system.

Status Indicator panel on Operator Control Box: under Emergency Stop button.



Status Indicator panel on machine: front right and left cover



CHAPTER 4: Calibration and Quality Assurance (QA) Procedures

Calibration Procedures

Calibrations are necessary for proper performance of the PedCAT. When calibration is required, a pop up message will appear during the start up screen for the Acquisition software and the service light will be illuminated. When this occurs, there will only be a limited number of days in which the machine will be operational without a current calibration.

Additionally, there are some calibration procedures that should only be run by a factory trained technician. These can be found in Appendix IV of this document.


Once the pop up message in Acquistion alerts the user that a Calibration is needed, the user can exit the Acquisition software and start up the CB-ToolShed software, located on the desktop of the Acquisition terminal. Once the CB-ToolShed software is started, a startup screen similar to Acquisition will be displayed.

DataBase	Institution Nar	me		
	Production Serial Number		Starting the Peo	dCAT Acquisition System
Dicom	1041 Dicom Connec	-	11	PedCAT May 2015
	Connected		1	May 2015
Firmware	Address 192.168.3.2 Count	Min Ver 10 Current Ver	C	Manufacturer: CurveBeam, LLC 175 Titus Avenue Suite 300 Warrington, PA 18976
Gantry	1017283	10.5	For technical sup	oport or questions contact CurveBearn at 267-483-8081
Globals	XPS Version 1 Last Gain Calib 6/9/2015 6:23		CurveBeam Europe, Ltd. Devonshire House 1 Devonshire Street London W1W 5DR, UK	Reference data provided under License by CurveBeam. LLC All Rights Reserved.
Panel	0, 5, 2015 0.25	-12 (11)	66	
Gantry Park	Imager C:\IMAGERs\I Panel Code 0	E523-11	C E 0473	
-	Temp 60 -	C Ma	tion.	
Temperature	40- 20- 0- C			
		Acc	quisition Version	

As CB-ToolShed starts up and checks all of the parts of the system, lights should change from red to green to indicate that the scanner is able to be used for calibrations, as shown below:

DataBase	Institution Name	
	Production Serial Number	Starting the PedCAT Acquisition System
Dicom	1041 Dicom Connect	PedCAT May 2015
	Connected	
Firmware	Address Min Ver	Manufacturer: CurveBeam, LLC 175 Thus Avenue
	192.168.3.2 10 Count Current Ver	Suite 300 Warrington, PA 18976
Gantry	1017283 10.5	For technical support or questions contact CurveBeam at 267-483-8081
	XPS Version	EC REP CurveBeam Europe, Ltd. Devonshire House
Globals	Last Gain Calibration 6/9/2015 6:23:19 AM	Devonsme House All Rights Reserved. 1 Devonshire Street London WIW 5DR, UK
Panel	_	
	Imager C:\IMAGERs\E523-11 Panel Code	
Gantry Park	0	
	Temp 60-36 C	tion:
Temperature	40-	
	20 20 c	OpenDoors
	Acc	auisition Version


Once all of the lights are green, then CB-ToolShed will appear as follows:

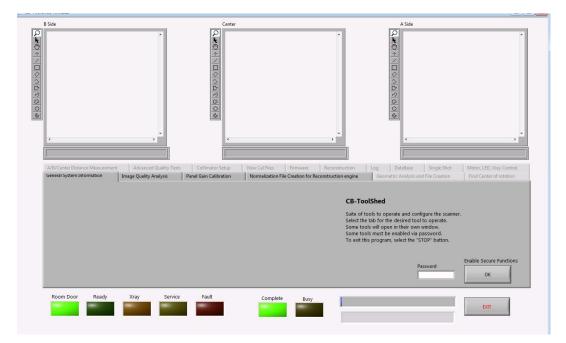


The first calibration that needs to be performed is the Panel Gain Calibration.

Panel Gain Calibration

Click on the tab for Panel Gain Calibration and the following will appear:

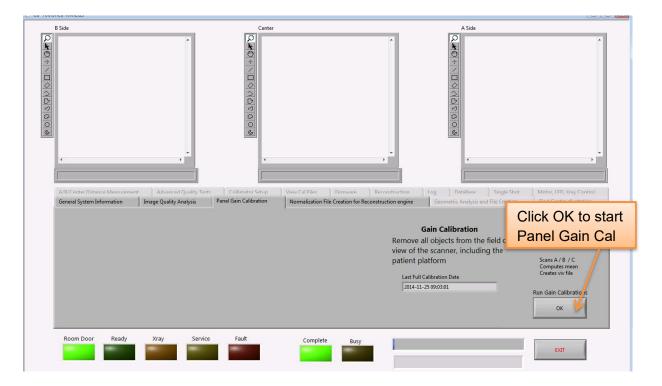


Before starting the Panel Gain Calibration, **ensure all objects are out of the field of view**, **including the patient platform**. To start the Panel Gain Calibration, click on the OK button under "Run Gain Calibrations." This will open the following screen:

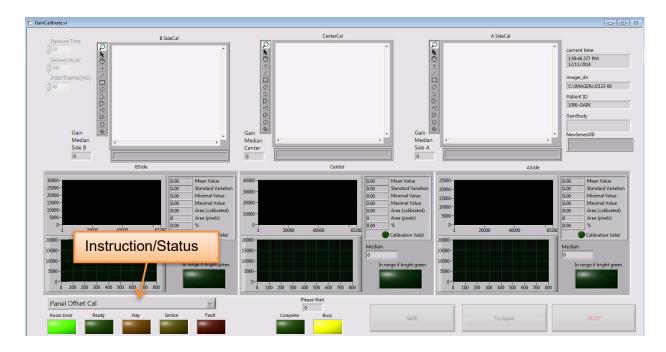

The user will receive messages and updates on what is happening as well as instructions on what to do (when to fire x-ray) in the window on the lower left corner. There will be a message to fire x-ray to perform the gain calibration on A Side. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

Once the x-ray has completed, release the scan button. The image on the screen will look similar to the below image where the A SideCal will now show an image of the empty panel as part of the calibration:

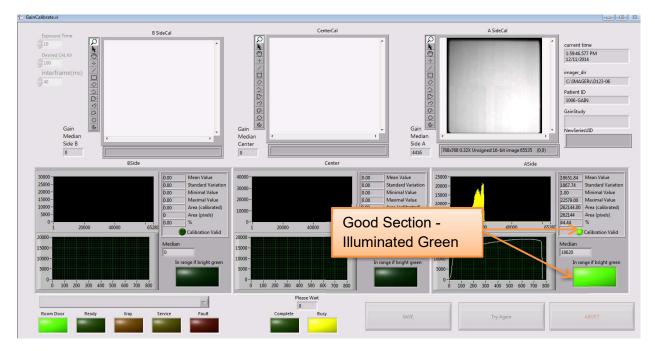


If the section was successful, there will be 2 green lights illuminated under the calibration side that was completed to show a successful 1/3 of the Panel Gain Calibration. Both the Calibration Valid and "In range if bright green" will illuminate bright green for a successful portion of the gain calibration as shown in the above picture. If the section was not successful, the lights will remain unilluminated.

After the A Side is completed, the B Side will need to be done. Instructions in the lower left corner will indicate when to fire the x-ray for the B Side. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

Once the x-ray has completed, release the scan button. The image on the screen will look similar to the below image where both A SideCal and B SideCal will now show an image of the empty panel as part of the calibration:

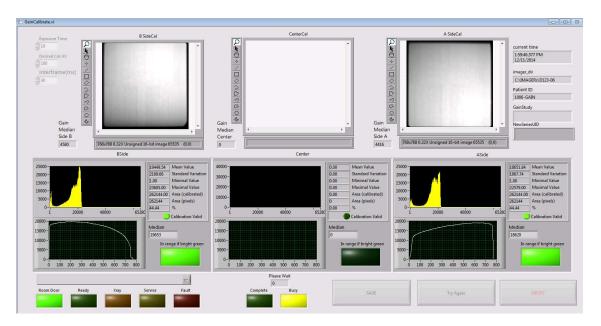


The B SideCal will now also show if the Calibration was valid or not, by illuminating the green lights for success and not illuminating them for failure. The lights for success or failure are same for all three calibration sections.

After the A and B sides are completed, the CenterCal will need to be run, the same as A and B side. Instructions in the lower left corner will indicate when to fire the x-ray for the CenterCal section. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure


Once the x-ray has completed, release the scan button. The image on the screen will look similar to the below image where all three will now show an image of the empty panel as part of the calibration as shown below:

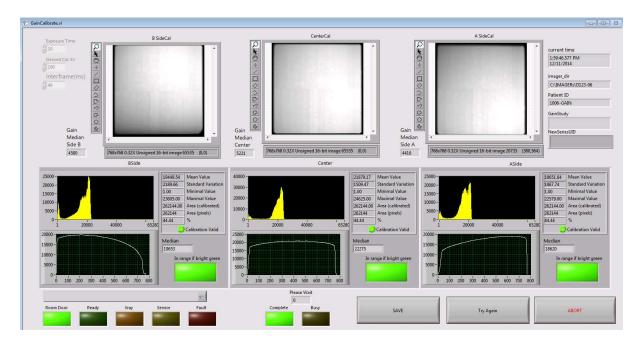


As for the A and B sides, the two green lights indicate success for the Center Cal, unilluminated lights indicate failure. In the image above, all three sections have passed successfully.

Once all 3 calibration scans have been taken, the three buttons in the lower right, SAVE, Try Again, and ABORT, will all become active and selectable. If all three sections had valid calibrations (all illuminated green) then select SAVE to save the values of the Panel Gain Calibration. If any section is not illuminated bright green there are two options. The first option is to select "Try Again" and run through the calibration another time. This can be done repeatedly. It is important if the user realizes something was left in the FOV and therefore will cause a failed section or more. The second option for a failed calibration is to select ABORT. This will revert back to the last good values before this calibration was run. These values will be able to be used for 21 days before a message appears on the Acquistion start up that will tell the user to run the calibrations again.

After the Panel Gain Calibration is completed successfully and SAVE is selected, the following pop up message will appear:

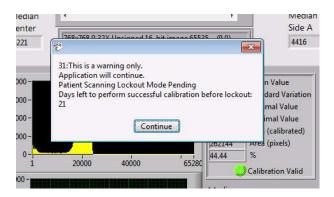


This message just indicates that there is more yet to do for the required calibrations, click Continue. Then another pop up message will appear as follows:

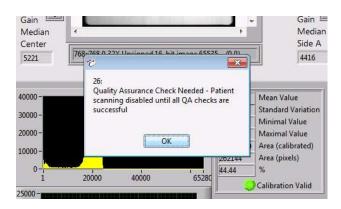

This one also is indicating that additional things need to be run, in this case, the Quality Assurance Check is needed, eventually. Click OK.


This will bring the user back to the Panel Gain starting point with another message to read as follows:

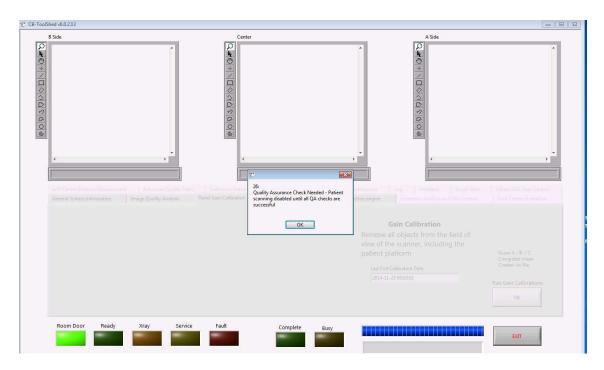


This message indicates also that Quality Assurance checks are still needed as a result of having changed the Panel Gain Calibration. Click OK.

Air Normalization Calibration


Then click on the "Normalization File Creation for Reconstruction engine" tab to start the Air Normalization Calibration, which will appear as follows:

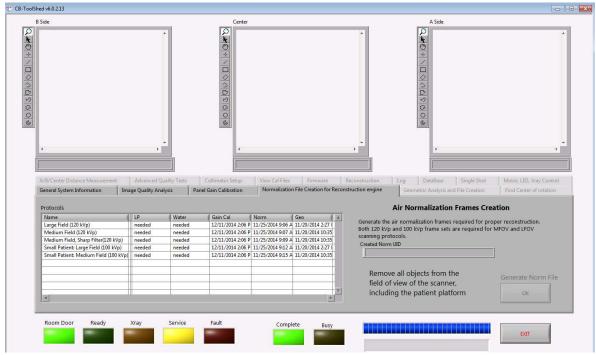

This calibration will create a norm file for each of the protocols listed. In order to do this, a scan must be taken using each protocol. **Ensure that there is nothing in the FOV, including the patient platform.** To start, click on the first protocol in the list, which will appears as follows:

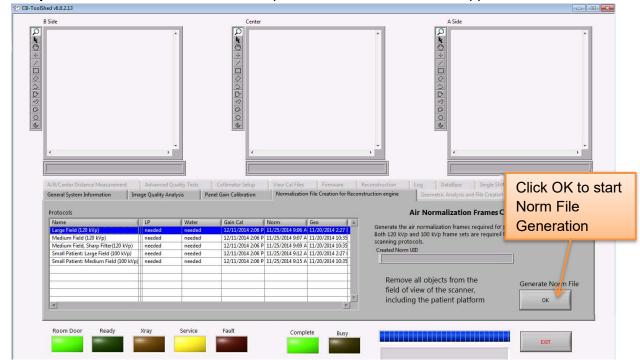

Once a protocol is selected, the OK button to "Generate Norm File" will be active and able to be selected. Select OK to start the norm file generation. During this process, it is normal for the screen to appear all washed out and be a light gray as below:

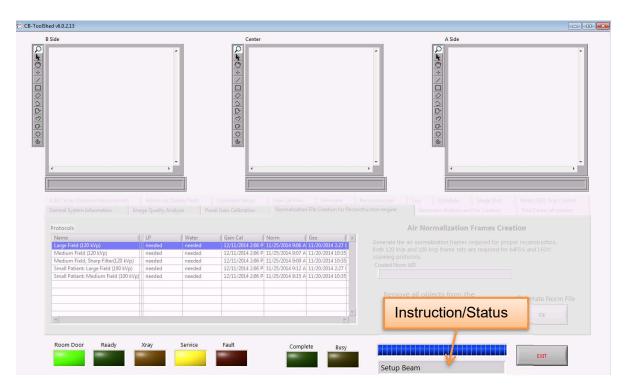


The software is processing and the progress can be seen by looking at the window in the lower right hand corner that displays the status and other user instructions, such as when to start the scan.

Instructions in the lower left corner will indicate when to fire the x-ray for the protocol selected. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure Once the x-ray has completed, release the scan button. For the LFOV scans, the x-ray will need to be fired twice, for the MFOV scans only once. After each scan is taken, a pop up message as shown below will appear:




Click OK to continue to the next protocol in the list. As each one is done, the current date and time will be entered in the Norm column with the protocol that was run, as shown below:

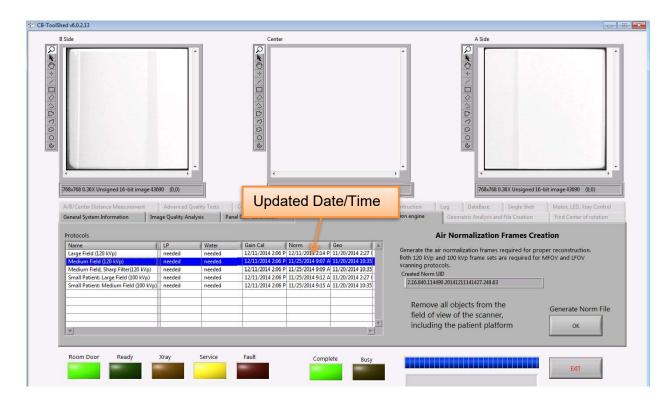

Continue with all of the protocols until each has an updated Norm date and time listed.

Image Quality Analysis – Line Pairs and Water

After all of the norm files have been created, click on the Image Quality Analysis tab and the following will be displayed:

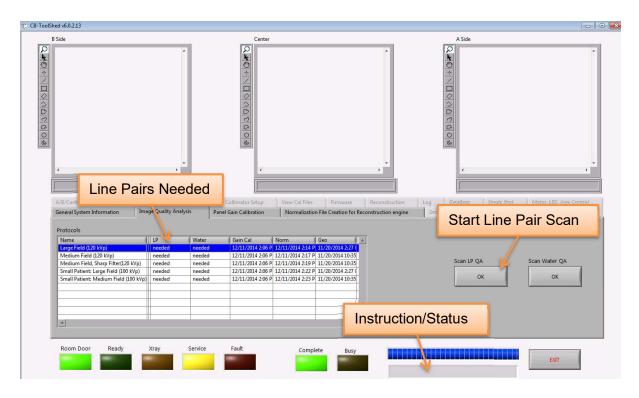

On this tab the Line Pair and Water QA scan dates are shown. In the image above, all of the Line Pair (LP) and Water QA scans still need to be done.

For these calibrations, the Line Pair phantom needs to be placed in the scanner. To do this, first place the Patient Platform in the scanner. Then place the Line Pair Phantom on the Patient Platform, using the circular positioning guides on the Patient Platform to center the phantom on the platform. The Line Pairs should run front to back on the machine, with the set of line pairs running Left to Right. Select a protocol that needs the Line Pair scan and then click the OK under "Scan LP QA" to start the scan.


Instructions in the lower right corner will indicate when to fire the x-ray for the protocol selected. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

48

Once the x-ray has completed, release the scan button. For the LFOV scans, the x-ray will need to be fired twice, for the MFOV scans only once.


The image of the phantom being scanned will be visible in the window at the top. If the user attempts the select the incorrect scan, there will be an error message after the scan is completed.

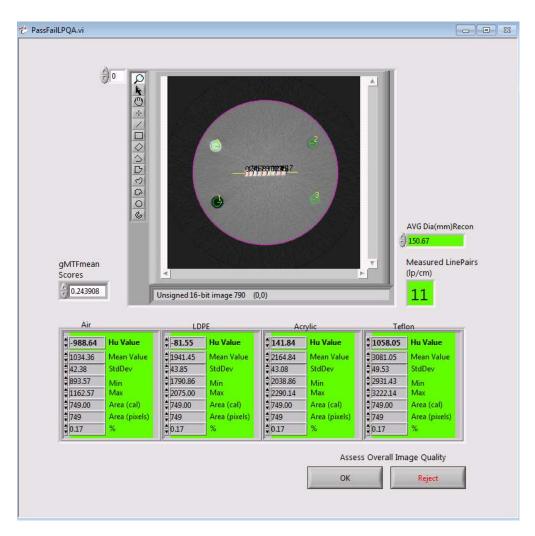

After the protocol is scanned, the following window pops up:

If all the colors are green, the values are good and the user should click the OK button. If the colors are red, the values are bad and the user should reject the scan. The user can then try the scan again, if the scan is continually rejected, then Technical Support should be contacted.

After the OK is selected, the following message will appear:



Select OK. Perform the remainder of the Line Pair scans. If the protocol has "needed" listed under the LP column, then that protocol still needs a LP scan. Once all of the entries in the LP column are filled in with date and times and no longer say "needed", remove the Line Pair Phantom from the scanner.


Remove the Line Pair Phantom from the scanner.

Place the Water Phantom in the center of the Patient Platform, using the circular positioning guides on the Patient Platform to center the water phantom on the platform. Perform a scan for every protocol listed with "needed" in the Water column of the table. Instructions in the lower right corner will indicate when to fire the x-ray for the protocol selected. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

Once the x-ray has completed, release the scan button. For the LFOV scans, the x-ray will need to be fired twice, for the MFOV scans only once.


The image of the phantom being scanned will be visible in the window at the top. If the user attempts the select the incorrect scan, there will be an error message after the scan is completed.

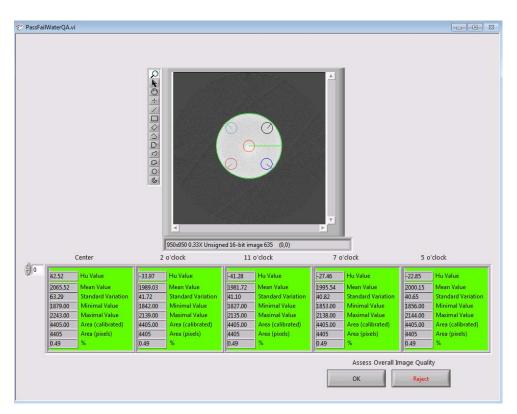

After the protocol is scanned, the following window pops up:

If all the colors are green, the values are good and the user should click the OK button. If the colors are red, the values are bad and the user should reject the scan. The user can then try the scan again, if the scan is continually rejected, then Technical Support should be contacted.

After the OK is selected, the following message will appear:



Select OK. Perform the remainder of the Water scans. If the protocol has "needed" listed under the Water column, then that protocol still needs a Water scan. Once all of the entries in the Water column are filled in with date and times and no longer say "needed", remove the Water Phantom from the scanner.

The User Calibrations are completed.

Advice: For additional calibrations, performed only by CurveBeam technicians, please refer to Appendix IV – Advanced Calibrations.

51

Quality Assurance Procedures

QA Test Procedures:


The QA test procedures are designed to check for Image Quality, Accuracy of Distance Measurements, and Consistency. These tests can be performed by a PedCAT owner/operator, or any service technician or radiation physicists. It is recommended that this QA test procedure be performed quarterly or if there are any indications of image quality or accuracy issues.


The QA tests will be performed by scanning specified QA phantoms provided by CurveBeam. These include a QA Line Pair/Chamber Phantom and a Water Phantom. Image Data will be captured and assessed for acceptable values For Assessments to be completed in CubeVue software, please refer to Post Processing of Data in Chapter 6 of this manual.

Image Quality (QA Phantom):

The items assessed for Image Quality will be:

- High Contrast Spatial Resolution measured via line pairs.
- Hounsfield Units (HU) accuracy of 4 Density chambers (Teflon, Acrylic, LDPE, Air)

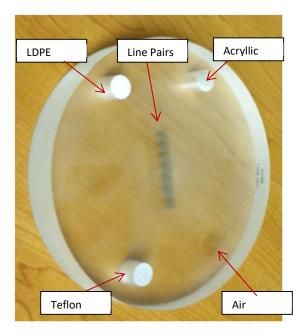

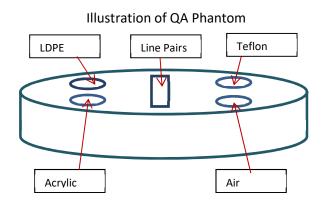

1. Place the QA Phantom on the devices patient platform using the circular positioning guides to center it on the platform.

2. Acquire a CBCT scan of the phantom using a Medium Field (120 kVp) scan option.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

Advice: Please refer to the Acquiring a Scan section of the manual, Chapter 6, for Acquiring the scan).

3. <u>Evaluate High Contrast Spatial Resolution</u>: Open the newly captured scan in CubeVue Viewing software and load the acquired scan to visually evaluate the line pairs for high contrast spatial resolution.

Advice: Please refer to Chapter 6 for instructions on use of CubeVue.


- a. Apply the Sharp Filter from within CubeVue keep this set for all of the remaining QA procedures.
- b. Change the slab thickness to the smallest thickness in the axial window keep this set for all of the remaining QA procedures.
- c. Observe the line pairs in the CubeVue Review/MPR Tab's axial view. (Refer to Chapter 6 for instructions on use of CubeVue). The axial image should be centered on the line pairs, use coronal and sagittal views to approximate the center of the line pairs (height), then view the line pairs in the axial window.
- d. The expected result should be 9 line pairs per cm or better. The line pairs start at 8 line pairs, so the second set of line pairs is 9 line pairs per cm, third set is 10 line pairs per cm, and so forth.
- *e.* Visually verify that there is definition present for each of the lines in pair 9 or higher.

4. Evaluate Hounsfield (HU) Accuracy:

a. On the axial view, measure the Hounsfield Units value of each density chamber. The results should fall within the below ranges.

Advice: Keep the HU circle off the borders of the chambers and use the small circles under the HU menu in CubeVue. Move the HU regions so that the first one on the list in CubeVue in the top right corner is the Air region, the second is Acrylic and continue around the circle. This then allows for the CubeVue top right HU Values to line up with the HU value order of the list below.

Density Material	Expected HU value Ranges
AIR (black chamber):	-1100 to -900
ACRYLIC (light gray chamber):	-50 to 200
LDPE (dark gray chamber):	-250 to -50
TEFLON (white chamber):	700 to 1200

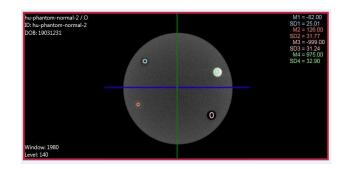

Distance Measurement Accuracy (QA Phantom):

Evaluate Distance Measurement Accuracy: In the currently open QA Phantom scan, Zoom into the Axial View's line pairs and make a distance measurement, using the Distance Tool, from one end of the line pair set to the other end of the line pair set. The distance should be between 41.0 - 42.5 mm.

Consistency/Uniformity (Water Phantom):

To evaluate consistency, we will image the Water Phantom. Water phantom image may vary from what was delivered with your machine.



- 1. The water phantom should be filled all the way to the top with distilled water, allow a bit of air space at the top to close the container.
- 2. Place the water phantom on the platform and ensure it is centered using the laser lights and circles on the patient platform.
- 3. Acquire a new scan of the water phantom using a **Medium Field (120 kVp) scan option**.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

Advice: Please refer to the Operations: Acquisition section of the manual, Chapter 6, for instructions on acquiring the scan.

- 4. Once the data is captured, it can be evaluated in the CubeVue, viewing software. Open the dataset to the Review/MPR Tab's Axial View. Apply the Sharp Filter and change the slab thickness on the axial window to the smallest possible slab size.
- 5. Noise Level Test: from the axial view, use the large Hounsfield circular measurements from within CubeVue and move them so that one is in the center of the water. <u>The Value should fall in the below range</u>: Water: -150 to 150
- 6. *Uniformity Test:* move the other 4 HU large circular measurements into the four quadrants, with the one from the prior step still in the center of the axial image. Note the Mean of each measurement. The mean of each quadrant measurement should be within 250 HU's from the center measurement mean.

Radiation Output Test:

It is recommended that a check of the kVp(eff) and Radiation Output of the X-ray source be performed annually by a qualified Physicist. The incident Absorbed Dose at the detector may be measured using a dosimeter. Tests are performed to assess output value and to check for tube output consistency and timer accuracy.

- 1. Attach a dosimeter to the detector such that the sensor is positioned where the vertical and lower horizontal laser lights intersect.
- 2. Perform a Standard scan of 20 cm diameter x 20 cm height, 0.3 voxel (Procedure Name: Medium Field (120kVp)) and record the time and dose from the meter.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

Advice: Please refer to the Operations: Acquisition section of the manual, Chapter 6, for instructions on acquiring the scan.


CHAPTER 5: Radiation Environment Survey

Scatter Measurements:

Methodology

Below is a diagram of where scatter measurements were taken. Scattered dose in the down direction could not be measured due to practical considerations of machine size, weight, etc. Dose in the down direction is conservatively assumed to be the same as in the up direction. This is considered conservative as machine structural components will attenuate the scattered beam significantly. For the lateral measurements, measurements were taken at a height of roughly 40 cm above the ground.

Two anthropomorphic foot phantoms were positioned in the center of the scanner. A Fluke 451p Ionization Chamber (SN# 2859 Calibrated 9/22/16) was used to measure the scattered radiation.

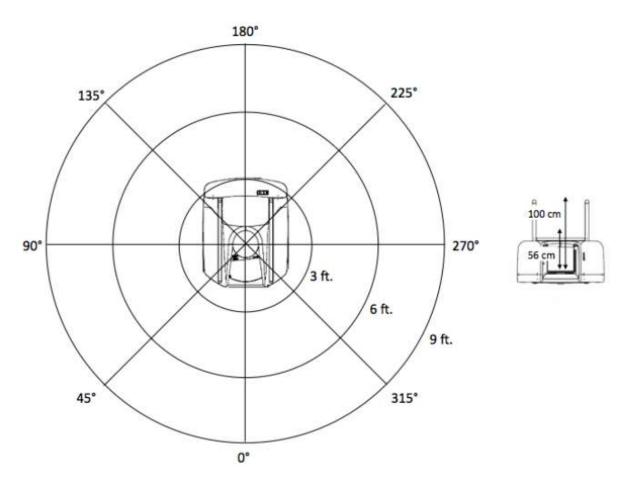

Scatter Measurements – Small Patient, Medium Field (100 kVp)

Unit:	PedCat	Mode:	Center, 2 foot phantoms in beam
Time:	16 sec	Field Size:	Medium
kVp:	100	mA:	5
Pulses:	377	Pulse Durati	ion: 0.012 sec

Location (Degrees)	Distance (ft)	Exposure (mR)	Exposure (µR)	Exposure (µR/mAs)	10 scans/week (mR/week)	25 scans/week (mR/week)	50 scans/week (mR/week)
	3	0.126	126	5.59	1.26	3.16	6.32
0	6	0.034	34	1.49	0.34	0.84	1.68
	9	0.014	14	0.62	0.14	0.35	0.70
	3	0.011	11	0.50	0.11	0.28	0.57
45	6	0.005	5	0.22	0.05	0.13	0.25
	9	0.002	2	0.07	0.02	0.04	0.08
	3	0.011	11	0.50	0.11	0.28	0.56
90	6	0.005	5	0.20	0.05	0.11	0.23
1000	9	0.001	1	0.04	0.01	0.03	0.05
3	3	0.006	6	0.28	0.06	0.16	0.31
135	6	0.001	1	0.04	0.01	0.03	0.05
	9	0.001	1	0.04	0.01	0.03	0.05
8 D	3	0.009	9	0.40	0.09	0.23	0.45
180	6	0.003	3	0.15	0.03	0.08	0.17
	9	0.001	1	0.04	0.01	0.03	0.05
	3	0.006	6	0.28	0.06	0.16	0.32
225	6	0.002	2	0.07	0.02	0.04	0.08
	9	0.001	1	0.03	0.01	0.02	0.03
	3	0.010	10	0.43	0.10	0.24	0.48
270	6	0.005	5	0.21	0.05	0.12	0.23
	9	0.001	1	0.06	0.01	0.03	0.07
	3	0.012	12	0.53	0.12	0.30	0.60
315	6	0.006	6	0.25	0.06	0.14	0.28
	9	0.003	3	0.15	0.03	0.08	0.17
1 m above	-	0.136	136	6.01	1.36	3.40	6.80

Scatter Measurements – Small Patient, Large Field (100 kVp)

Unit:	PedCat	Mode:	Center, 2 foot phantoms in beam
Time:	32 sec	Field Size:	Large
kVp:	100	mA:	5
Pulses:	754	Pulse Durati	on: 0.012 sec

Location (Degrees)	Distance (ft)	Exposure (mR)	Exposure (µR)	Exposure (µR/mAs)	10 scans/week (mR/week)	25 scans/week (mR/week)	50 scans/week (mR/week)
	3	0.220	220	4.86	2.20	5.50	11.00
0	6	0.063	63	1.39	0.63	1.58	3.15
	9	0.024	24	0.52	0.24	0.59	1.18
	3	0.020	20	0.44	0.20	0.50	1.00
45	6	0.009	9	0.21	0.09	0.23	0.47
	9	0.005	5	0.10	0.05	0.12	0.23
	3	0.018	18	0.40	0.18	0.45	0.90
90	6	0.006	6	0.13	0.06	0.15	0.30
	9	0.002	2	0.04	0.02	0.05	0.10
3	3	0.013	13	0.28	0.13	0.31	0.63
135	6	0.003	3	0.07	0.03	0.08	0.15
	9	0.001	1	0.02	0.01	0.03	0.05
· · · · · · · · · · · · · · · · · · ·	3	0.018	18	0.40	0.18	0.45	0.90
180	6	0.006	6	0.13	0.06	0.15	0.30
1100200	9	0.002	2	0.04	0.02	0.05	0.10
	3	0.011	11	0.24	0.11	0.27	0.53
225	6	0.003	3	0.07	0.03	0.08	0.15
	9	0.002	2	0.04	0.02	0.04	0.08
	3	0.017	17	0.38	0.17	0.43	0.85
270	6	0.009	9	0.20	0.09	0.23	0.45
2/0	9	0.002	2	0.05	0.02	0.06	0.12
6	3	0.021	21	0.47	0.21	0.53	1.07
315	6	0.011	11	0.25	0.11	0.28	0.57
0.000	9	0.009	9	0.19	0.09	0.22	0.43
1 m above		0.23	230	5.08	2.30	5.75	11.50

Scatter Measurements – Large Patient, Medium Field (120 kVp)

Unit:	PedCat	Mode:	Center, 2 foot phantoms in beam
Time:	16 sec	Field Size:	Medium
kVp:	120	mA:	5
Pulses:	377	Pulse Durati	on: 0.012 sec

Location (Degrees)	Distance (ft)	Exposure (mR)	Exposure (µR)	Exposure (µR/mAs)	10 scans/week (mR/week)	25 scans/week (mR/week)	50 scans/week (mR/week)
	3	0.230	230	10.17	2.30	5.75	11.50
0	6	0.054	54	2.40	0.54	1.36	2.72
	9	0.027	27	1.18	0.27	0.67	1.33
Ĩ	3	0.024	24	1.06	0.24	0.60	1.20
45	6	0.009	9	0.41	0.09	0.23	0.46
	9	0.005	5	0.24	0.05	0.13	0.27
	3	0.023	23	1.02	0.23	0.58	1.15
90	6	0.007	7	0.31	0.07	0.18	0.35
	9	0.004	4	0.19	0.04	0.11	0.21
	3	0.013	13	0.57	0.13	0.33	0.65
135	6	0.005	5	0.22	0.05	0.13	0.25
	9	0.002	2	0.09	0.02	0.05	0.10
	3	0.021	21	0.93	0.21	0.53	1.05
180	6	0.007	7	0.31	0.07	0.18	0.35
	9	0.003	3	0.15	0.03	0.08	0.17
	3	0.013	13	0.57	0.13	0.33	0.65
225	6	0.005	5	0.22	0.05	0.13	0.25
	9	0.002	2	0.09	0.02	0.05	0.10
	3	0.023	23	1.00	0.23	0.57	1.13
270	6	0.008	8	0.34	0.08	0.19	0.38
. Chever a	9	0.004	4	0.18	0.04	0.10	0.20
	3	0.029	29	1.27	0.29	0.72	1.43
315	6	0.009	9	0.40	0.09	0.23	0.45
	9	0.007	7	0.29	0.07	0.17	0.33
1 m above		0.23	230	10.17	2.30	5.75	11.50

Scatter Measurements – Large Patient, Large Field (120 kVp)

Unit:	PedCat	Mode:	Center, 2 foot phantoms in beam
Time:	32 sec	Field Size:	Large
kVp:	120	mA:	5
Pulses:	754	Pulse Durati	on: 0.012 sec

Location (Degrees)	Distance (ft)	Exposure (mR)	Exposure (µR)	Exposure (µR/mAs)	10 scans/week (mR/week)	25 scans/week (mR/week)	50 scans/week (mR/week)
	3	0.440	440	9.73	4.40	11.00	22.00
0	6	0.102	102	2.25	1.02	2.54	5.08
9	9	0.048	48	1.07	0.48	1.21	2.42
	3	0.041	41	0.90	0.41	1.02	2.03
45	6	0.018	18	0.40	0.18	0.45	0.90
	9	0.010	10	0.21	0.10	0.24	0.48
	3	0.044	44	0.97	0.44	1.09	2.19
90	6	0.014	14	0.30	0.14	0.34	0.68
1000	9	0.006	6	0.13	0.06	0.15	0.30
	3	0.023	23	0.51	0.23	0.58	1.16
135	6	0.009	9	0.20	0.09	0.23	0.45
-	9	0.003	3	0.07	0.03	0.08	0.15
	3	0.037	37	0.83	0.37	0.93	1.87
180	6	0.012	12	0.27	0.12	0.31	0.62
	9	0.006	6	0.13	0.06	0.14	0.28
	3	0.024	24	0.54	0.24	0.61	1.22
225	6	0.008	8	0.17	0.08	0.19	0.38
	9	0.003	3	0.07	0.03	0.08	0.15
	3	0.046	46	1.01	0.46	1.14	2.28
270	6	0.014	14	0.32	0.14	0.36	0.72
	9	0.009	9	0.21	0.09	0.23	0.47
	3	0.047	47	1.05	0.47	1.18	2.37
315	6	0.021	21	0.46	0.21	0.52	1.03
	9	0.013	13	0.29	0.13	0.33	0.67
1 m above		0.385	385	8.51	3.85	9.63	19.25

Scatter Measurement - 22" Directly above patient opening

This measurement was taken using the same Ion Chamber instruments noted above but located 22 inches above the patient platform which correlates to the smallest patient's groin location. Two foot phantoms were located in the patient opening for this measurement.

Mode	kVp	mAs	Distance (in)	Exposure (mR)
Small Patient Medium Field	100	22.62	22	0.71
Small Patient Large Field	100	45.24	22	1.20
Large Patient Medium Field	120	22.62	22	1.19
Large Patient Large Field	120	45.24	22	2.0

CTDI:

Small Patient (100 kVp) – Medium View

Without AEC

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	100	8
mA	5	
Beam Width at Isocenter (mm) ¹	209.51	
Center		
Average of center measurements (mR)		83.6
CTDI at isocenter in phantom (mGy)	į.	0.727
12 o'clock position		
Average of 12 o'clock measurements (mR)		100.43
CTDI at 12 o'clock position in phantom (mGy)		0.874
CTDIw and CTDIvol (mGy)	v.	0.825
DLP (mGy-cm)	=CTDIvol*20.951	17.3

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	100	
mA	5	
Beam Width at Isocenter (mm) ¹	209.51	
Center		
Average of center measurements (mR)	й Г	75.2
CTDI at isocenter in phantom (mGy)		0.654
12 o'clock position		-
Average of 12 o'clock measurements (mR)		85.65
CTDI at 12 o'clock position in phantom (mGy)		0.745
CTDIw and CTDIvol (mGy)		0.715
DLP (mGy-cm)	=CTDIvol*20.951	15.0

CTDIvol Without AEC	CTDIvol With AEC	Percent Difference
0.825 mGy	0.715 mGy	13.35

Small Patient (100 kVp) – Large View

Without AEC

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	100	
mA	5	
Beam Width at Isocenter (mm) ¹	209.51	
Center		
Average of center measurements (mR)		132.9
CTDI at isocenter in phantom (mGy)		1.156
12 o'clock position		
Average of 12 o'clock measurements (mR)		128.0
CTDI at 12 o'clock position in phantom (mGy)	4 5	1.114
CTDIw and CTDIvol (mGy)		1.128
DLP (mGy-cm)	=CTDIvol*20.951	23.6

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	100	
mA	5	
Beam Width at Isocenter (mm) ¹	209.51	
Center		
Average of center measurements (mR)		116.7
CTDI at isocenter in phantom (mGy)	2	1.015
12 o'clock position		
Average of 12 o'clock measurements (mR)		107.3
CTDI at 12 o'clock position in phantom (mGy)	in the second	0.934
CTDIw and CTDIvol (mGy)		0.961
DLP (mGy-cm)	=CTDIvol*20.951	20.1

CTDIvol Without AEC	CTDIvol With AEC	Percent Difference
1.128 mGy	0.961 mGy	14.8%

Large Patient (120 kVp) – Medium View

Without AEC

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	120	
mA	5	1
Beam Width at Isocenter (mm) ¹	209.51	
Center		
Average of center measurements (mR)		139.5
CTDI at isocenter in phantom (mGy)		1.213
12 o'clock position	· /	
Average of 12 o'clock measurements (mR)		161.1
CTDI at 12 o'clock position in phantom (mGy)	1	1.402
CTDIw and CTDIvol (mGy)		1.339
DLP (mGy-cm)	=CTDIvol*20.951	28.1

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	120	
mA	5	
Beam Width at Isocenter (mm) ¹	209.51	
Center		
Average of center measurements (mR)		119.4
CTDI at isocenter in phantom (mGy)	-	1.039
12 o'clock position		
Average of 12 o'clock measurements (mR)	÷	134.8
CTDI at 12 o'clock position in phantom (mGy)		1.173
CTDIw and CTDIvol (mGy)		1.128
DLP (mGy-cm)	=CTDIvol*20.951	23.6

CTDIvol Without AEC	CTDIvol With AEC	Percent Difference
1.339 mGy	1.128 mGy	15.7%

Large Patient (120 kVp) – Large View

Without AEC

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	120	5
mA	5	
Beam Width at Isocenter (mm) ¹	209.51	
Center	8	ŧ.
Average of center measurements (mR)	9. 15	223.3
CTDI at isocenter in phantom (mGy)	4	1.943
12 o'clock position		
Average of 12 o'clock measurements (mR)	ф.	215.9
CTDI at 12 o'clock position in phantom (mGy)	8. 4 .	1.879
CTDIw and CTDIvol (mGy)		1.900
DLP (mGy-cm)	=CTDIvol*20.951	39.8

CTDI Head Phantom (16-cm diameter PMMA phantom)	Measured	Calculated
kVp	120	
mA	5	
Beam Width at Isocenter (mm) ¹	209.51	-
Center		
Average of center measurements (mR)	a.	190.6
CTDI at isocenter in phantom (mGy)	9. 4	1.658
12 o'clock position		
Average of 12 o'clock measurements (mR)		180.6
CTDI at 12 o'clock position in phantom (mGy)	1 .	1.571
CTDIw and CTDIvol (mGy)	k:	1.600
DLP (mGy-cm)	=CTDIvol*20.951	33.5

CTDIvol Without AEC	CTDIvol With AEC	Percent Difference
1.900 mGy	1.600 mGy	15.8%

Z-axis point spread function:

The pedCAT has a fixed and rigid patient positioning platform that does not incorporate any table motion or indexing (no "table pitch"). The detector panel has a square shape, while the pixels on the panels are square shaped as well. The raw projections are acquired in a single 360 degree orbit, thus covering the entire Field of View (FOV) height in one rotation. This results in isotropic voxels in the reconstructed volume, hence the same spatial resolution in the z-axis as in the x-y plane. Due to this projection geometry, calculation of a separate z-axis point spread function should not be applicable.


Recommended Operating Requirements:

Local agencies or government bodies or international standards may dictate requirements for installation of the system in order to protect personnel and the public from exposure from the radiological output of the device. Consult your local agencies, government bodies, or international standards for actual requirements which apply.

It is recommended that a qualified Physicist or Radiologist determine where appropriate, the applicable lead shielding to be installed in the area around the system equipment. Below are some other common requirements that may apply to your location:

- The Operations computer (server) and X-ray Operator should be located behind a properly shielded permanent barrier. A viewing window should be present to enable the X-ray Operator to view the Patient and operate the computer while the exposure is present.
- Operators should consider the use of a lead apron to protect the anatomical areas of the medical personnel working in the areas exposed to radiation.
- The Operator Control Box and Acquisition Computer shall be located within 1 meter [3.28 ft] from a door. If not, an interlocked door may be required.
- A room door may be required.
- Radiation warning signs may be required next to the entrance to the room.
- A Warning light may be required by the entrance to the room.
- A shielding plan should be performed where the system is being installed. Some local agencies or government bodies require that a shielding plan be conducted by a qualified Physicist or Radiologist and a copy of the shielding plan be submitted and approved prior to installation of the system.
- An area radiation survey by a qualified physicist or Radiologist may then be required within 30 days of initial clinical use of the system. This survey may be required to be submitted to the local agency or government body

66

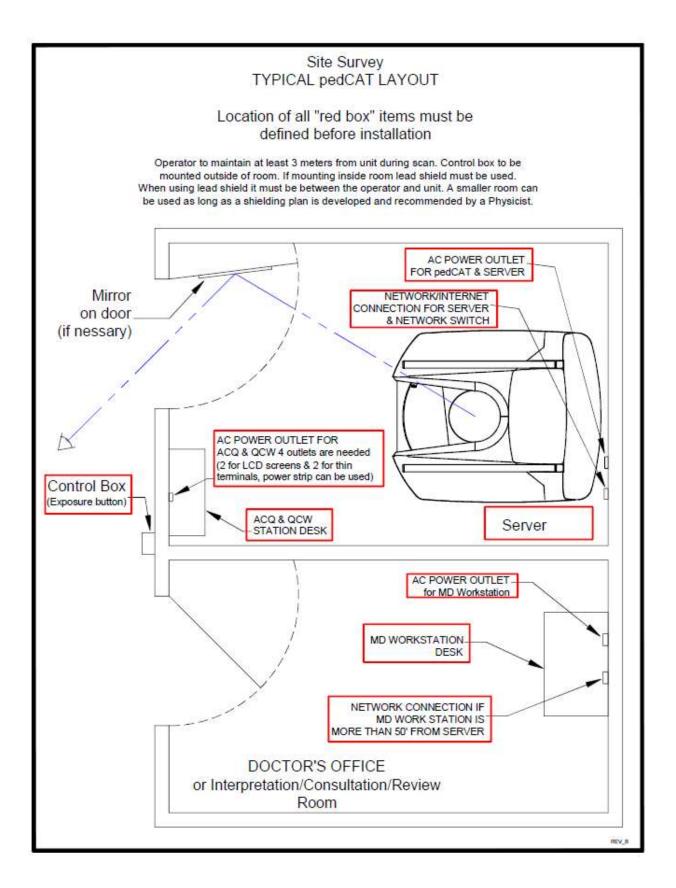

Effective Dose to Patient Measurements (Micro Sieverts):

Effective Dose in Micro Sieverts (µSv)
1-2
1 - 2
4 - 7
4 - 7
2 - 3
3 - 5
2 - 3
3 - 5
5 - 9
9 - 14
5 - 9
9 - 14

Report on CurveBeam CBCT Foot Dosimetry John Ludlow, DDS, MS, FDS RCSEd

Methods:

A custom tissue equivalent anthropomorphic phantom of the foot and ankle was constructed (The Phantom laboratory, Salem, NY). The model was constructed in 25 mm horizontally sliced layers allowing separation and specific localization of dosimeters within each layer.

Slots were drilled in the upper surface of the layers to accommodate placement of NanoDot OSL dosimeters. Slots were located in and on tissues included in the weighted tissues used in the 2007 ICRP calculation of effective dose. Twenty-one dosimeter locations were utilized.

X-ray Tube Assembly:


CurveBeam utilizes an X-ray Tube, model SXR 130-20-0.5, from Superior X-ray Tube Co, 1220 Claussen Drive, Woodstock, IL 60098. Below are the X-ray Tube Specifications:

Superior X-ray Data for the SXR 130-20-0.5:

SXR 130-20-0.5

The SXR 130-20-0.5 insert is a stationary anode, glass envelope x-ray tube. The SXR 130-20-0.5 is an x-ray tube originally designed for use in dental CBCT* applications. The insert should be housed in a unit that allows for insulating media such as high dielectric mineral oil (Diala-AX) or high dielectric pressurized gas such as SFo (Sulfur Hexafluoride).

* Cone Beam Computerized Tomography

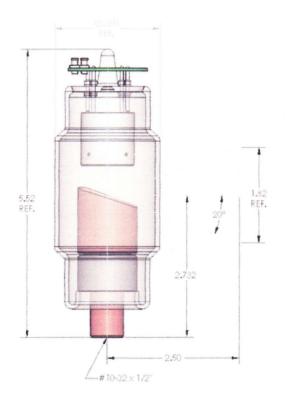

SXR 130-20-0.5 Outline Drawing

Physical Characteristics:

Glass Frame: Inherent Filtration:

Focal spot: Target Angle: Target Material: Filament Material: Focus Cup Material: Anode Body: Borosilicate 0.085 thick: 1.1 mm Al equivalent at 80 kV 0.5 mm Nominal 20° Tungsten Tungsten Nickel Copper


Thermal Characteristics:

Anode Heat Storage	
Capacity:	30 KHU's (21KJ)
Max Anode Heat	
Dissipation Rate:	17.9 KHU's/min.
Duty Cycle:	1:20


Electrical Characteristics:

Max. Tube Potential:	130 kV
Filament V-A Curve:	See Chart
Max. Power:	See Chart
Max Single exposure	See Chart
Max. Continuous Exp.	1.8 mA

NOTE: * P/ease contact Superior Engineering Department for cathode terminations options.

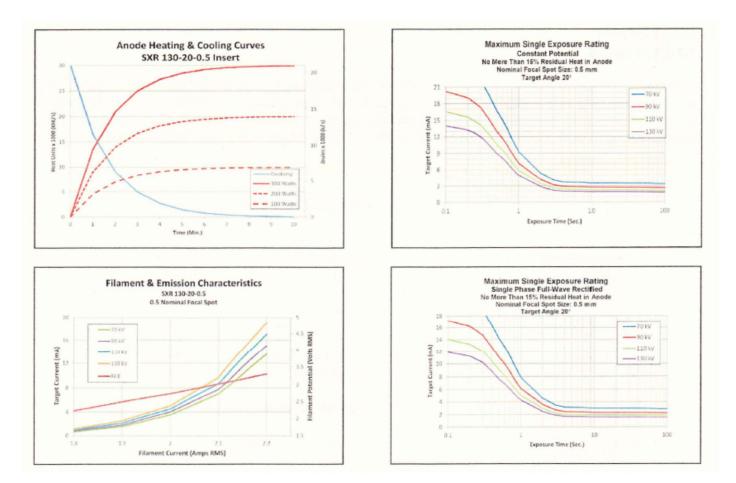

Beam Path and Angulation:

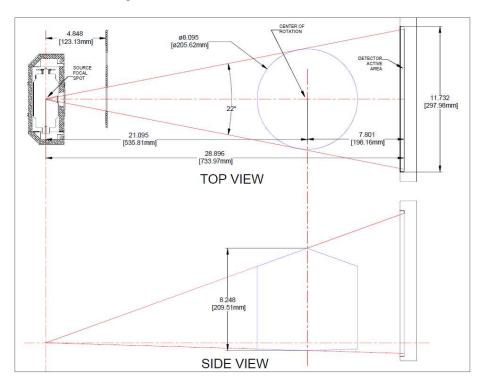

CHAPTER 6: Operations - Acquiring a Scan

ACQUIRING A SCAN

System Startup:

The PedCAT system at a minimum includes the Scanning device, the computer server, and an Operator's control Terminal. All must be powered **ON** in order for the system to operate properly.

The Scanning device circuit breaker should always be set to the ON position. This is located in the back of the machine. This is the machine ON/OFF control. The vertical line is the ON position. The 0 is the OFF position. The image below shows the scanner in the ON position:



Power ON is indicated on both the Machine Status Indicator panel and the Operators control box Status indicator panel lights. Power ON is lit in **Green**. The machine must be ON for 30 seconds before the Acquisition Software should be launched. Optimal Scanning results will be achieved with the machine warmed up for 2 hours.



The scanning software is accessed via the Quality Control Workstation (QCW) and can be viewed on the DELL tower as well.


Start up the Acquisition software by double clicking on the CB-Scanner Shortcut




An "About Screen" will appear which displays the software version number and details. Or, the following About screen can always be accessed from the Acquisition software's "About" button.

Fo	Curvel 175 Tri Suite 3 Warrin	6.0.4.7	
CurveBe Devonsh 1 Devons	am Europe, Ltd. Referen CurveE	nce data provided under License by learn. LLC nts Reserved.	
C	0473		
C	0473 Additional Information		
C		Version	11
C	Additional Information	Version A Revision L07 Build 029	
C	Additional Information		
C	Additional Information Filename VirtCp.dll	Revision L07 Build 029	
	Additional Information Filename VirtCp.dll DicomObjects.ocx	Revision L07 Build 029 v4.1	
C	Additional Information Filename VirtCp.dll DicomObjects.ocx dcm4chee-psql	Revision L07 Build 029 v4.1 2.17.1	

Once the acquisition software is launched, a system "Startup" window (also referred to as the "Initialization" window) will display indicating if various parts of the system are functioning properly or not. When the row has two dark buttons, that item is still awaiting a status and will eventually change the color from either the dark green to bright green or from dark red to bright red. The bright red buttons can indicate the functionality is still undergoing the startup test, so until it has successfully passed this testing, it will be illuminated bright red.

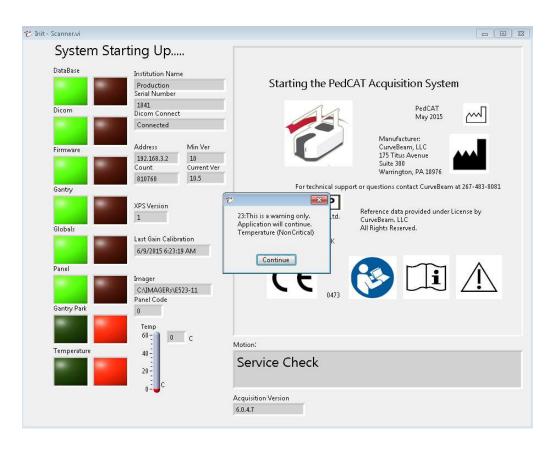

If one of more of these functions illuminates bright red, and remains bright red, it indicates a failure, please contact CurveBeam Technical Support if a light REMAINS on as follows:

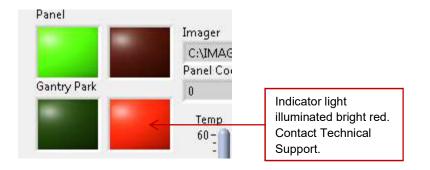

All Startup lights should be illuminated bright green once diagnostics have been completed successfully. If Startup was successful, the Startup window will close on its own, and the software will automatically display the Patient Worklist Window. The following depicts a successful Startup with all lights illuminated bright green:

DataBase				
	Institution Nan Production	ne	Starting the Ped	ICAT Acquisition System
	Serial Number		starting the rea	is try tequisition system
Dicom	1041		10	PedCAT 🗖
	Dicom Connec Connected	.t		May 2015
	Connecteu			Manufacturer:
Firmware	Address	Min Ver		CurveBeam, LLC
	192.168.3.2	10		175 Titus Avenue Suite 300
	Count 810760	Current Ver 10.5		Warrington, PA 18976
Gantry	810/00	10.5	For technical sup	port or questions contact CurveBeam at 267-483-8081
	-		EC REP	
	XPS Version		CurveBeam Europe, Ltd.	Reference data provided under License by
Globals	-		Devonshire House	CurveBeam. LLC All Rights Reserved.
	Last Gain Calib	ration	1 Devonshire Street London W1W 5DR, UK	
	6/9/2015 6:23:	19 AM		
Panel			~ ~	
	Imager		CE	
	C:\IMAGERs\E	523-11	0473	
Gantry Park	Panel Code			
	Temp 60-133	T _c		
Temperature		Mo	tion:	
	40-	C	DpenDoors	
	20- 0-C		spendoord	
	- c			

PedCAT Acquisition Software Interface:

The PedCAT Acquisition Software, "CB Scanning Device" Interface consists of the below sections, each with its own tab near the top of the screen:

- <u>Patient List:</u> Access or Add New patient information and intended procedure.
- <u>Procedure</u>: Perform the Scan Acquisition.
- <u>Quality</u>: Perform a QA (Quality Assurance) check of the scan acquired.

PATIENT LIST: Accessing/Entering Patient Information & Selecting Scan Procedure:

Patient Demographic Information can be either imported into the system via a Worklist or can be Added as a "New Patient" via the PedCAT ACQ software Patient Tab when "Add Patient" is selected.

orklist						Protocol Selection				
Patient Name	^Patient ID	^Accession	^BirthDate	^ScanDate		Name	Code	Description		
nifer Jackson	JAK1235	129	19800315	20131020		Large Field (120 kVp)	A-CBCTLF120	Extended Diameter, 35D	x 20H, 120 kVp	
						Medium Field (120 kVp)	B-CBCTMF120	20D x 20H, 120 kVp		
						Medium Field, Sharp Filter(120 kVp)	C-CBCTMF120S	20D x 20H, 120 kVp Shar	р	
						Small Patient: Large Field (100 kVp)	D-CBCTLF100	Under 100 pounds, Exter	nded Diameter, 3	35D x 20H, 100
					-	Small Patient: Medium Field (100 kVp)	E-CBCTMF100	Under 100 pounds, 20D :	x 20H, 100 kVp	
					7					
ame						Protocol Details		(Value	Dicom	0 0 0
		cian Name	¥	cheduled Time /		×	vi	BOUT buttor ewing softwa ersion & deta	are	A

To add a patient's scan to the Worklist, select the "Add Patient" button at the bottom of the screen. If a procedure is added by mistake or needs to be removed, highlight the entry in the worklist and select the "Remove Patient" button at the bottom and the patients scan will be removed from the list.

When the "Add Patient" button is selected, the following pop up box will appear for patient information to be added:

PatientID		Requesting Physician Name		
Johnson12345		Michaels		
PatientName(last, first)		BirthDate		Gender
Johnson, Robert		2/28/1970	C	Male 🤝
Accession Number				
511		Clear Patient Data		
Procedures To Add				
Procedure	Code	Description		-
CT LE LEFT WITHOUT CONTRAST	CTLELWO			
CT LE LEFT WITH CONTRAST	CTLELW			
CT LE RIGHT WITHOUT CONTRAST	CTLERWO			
CT LE RIGHT WITH CONTRAST	CTLERW			
CT LE BILATERAL WITHOUT CONTI	R CTLEBWO			
CT LE BILATERAL WITH CONTRAST	CTLEBW			
CT FOLLOWUP	CTFU STY			
Add	1.	" Cancel		

On the Add Patient Procedure window, the minimal patient information that MUST be entered is **Patient ID, Patient Name and Procedure To Add. The ID# MUST be unique to this patient**. The other items are optional. The Accession Number field can be manually entered, or if left blank one will be auto generated. After all the required fields are entered and any optional fields as well, select the "OK" button under "Add" to add the patient to the Worklist.

To select the patient for the scan, highlight on the patient's line in the Worklist. The patient's information that was entered will appear under the worklist. Select a protocol from the right side of the screen, under Protocol Selection, for the list provided. The details of the protocols are listed below the Protocol Selections, as each one is selected. Once the patient and protocol have been selected, click on "Accept/Next" to move to the Procedure tab. The "Accept/Next" button is remain grayed out until the patient and protocol have both been selected.

Patient Procedure Quality	
Worklist	Protocol Selection
APatient Name Apatient ID Accession ABirthDate VScanDate	Name Code Description
Johnson, Robert Johnson12345 511 19700228 20150624	Large Field (120 kVp) A-CBCTLF120 Extended Diameter, 35D x 20H, 120 kVp
· · · · · · · · · · · · · · · · · · ·	Medium Field (120 kVp) B-CBCTMF120 20D x 20H, 120 kVp
	Medium Field, Sharp Filter(120 kVp) C-CBCTMF120S 20D x 20H, 120 kVp Sharp Small Patient Large Field (100 k/m) D_CBCTL5300 Linder 130 pounds, Extended Diameter, 35D x 20H, 100 kV
Patient Highlighted	Small P trees Lives Field 200 kgs December 200 Lived 200 pounds, Extended Diameter, 350 x 20H, 100 ky Small P. Select Protocol to Perform
Patient Information Displayed	
Name	Protocol Details Value Dicom
Johnson, Robert Patient ID Johnson 1245 BithDate Gender StepID Accession Scheduled Time 19700228 M S198 511 20150624 / 1205 Procedure	B - CBCTMF120200 2:0H, 120 KVp M - MedumVolumeVMIRAFRormats:MNR1-55-20 M - AX-FULL1: M - AX-FULL1: M - AX-FULCED:3 M - CR-REDUCED:4
CT LE LEFT WITHOUT CONTRAST/CTLELWO	T
UID Ref Physician Name 21.6.840.114490.20150624120529.364.2 Michaels Add Patient Remove Patient	ABOUT
Room Door Ready Xray	Service Fault Accept / Next -> Accept/Next

Patient Size for Protocols :

Patient size has been separated into 2 categories

- Small size (this will use exposure factors of 100 kVp, 5 mA).
- Normal to Large size (this will use exposure factors of 120 kVp, 5 mA).

Small is defined as patients weighing 100 pounds (45 kg) or less, with a minimum weight of 50 pounds (23 kg) and groin area at least 22" (56 cm) above the floor.

Normal to Large is the remaining population which is defined as 101 - 400 pounds (46 - 181 kg) and groin area at least 22" (56 cm) above the floor.

RECOMMENDATIONS for Selecting a Protocol:

There are 5 Protocols to select from:

Medium Field (120kVp): (20 cm diameter x 20 cm height, 0.3 voxel):

Select this option if the patient size is normal-large as defined above, and if you need to capture only one foot or a partial area of interest for one foot.

<u>Medium Field, Sharp Filter (120kVp):</u> (20 cm diameter x 20 cm height, 0.3 voxel): Select this option if the patient size is normal-large as defined above, and if you need to capture only one foot or a partial area of interest for one foot, but specifically for visualizing anticipated small fractures or stress fractures.

Large Field (120kVp): (35 cm diameter x 20 cm height, 0.37 voxel):

Select this option if the patient size is normal-large as defined above, and if you need to capture both feet in a scan. This procedure automatically executes 2 rotations around the patient so it is longer than the single foot procedure.

<u>Small patient: Medium Field (100kVp):</u> (20 cm diameter x 20 cm height, 0.3 voxel):

Select this option if the patient size is small as defined above, and if you need to capture only one foot or a partial area of interest for one foot.

Small patient: Large Field (100kVp): (35 cm diameter x 20 cm height, 0.37 voxel):


Select this option if the patient size is small as defined above, and if you need to capture both feet in the scan. This protocol automatically executes 2 rotations around the patient so it is longer than the single foot procedure.

WARNING The patient must wear a protective full wrap X-ray shielding apron (lead apron) during a scan. Patients less than 21 years old, small size patients (under 100 pounds) and children must also wear a gonad and ovarian front and back protective shield.

Once the Protocol is highlighted, the "Accept/Next" button will become non-gray. Click "Accept/Next" when the protocol is correct for the patient being scanned to continue with the Acquisition process.

PROCEDURE: Performing the Acquisition:

The Acquisition will be performed via the "Procedure" Tab. The Procedure Tab will display the current selected Patient Name and Procedure, as well as User Instructions and Information as to the status of what the software and scanner are doing.

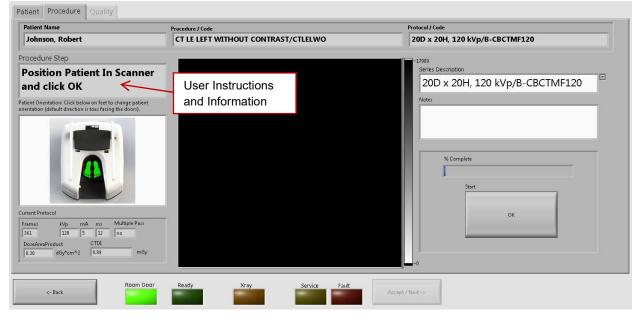

Follow the instructions as stated in the Procedure Step box.

Additionally if an alternate Series Description is desired, select from the pulldown list, or use the blank entry to provide a different Series Description.

Patient Name	Procedure / Code	Protocol / Code
Johnson, Robert	CT LE LEFT WITHOUT CONTRAST/CTLELWO	20D x 20H, 120 kVp/B-CBCTMF120
ocedure Step		
Position Patient In Scanner		-17000 Series Description
nd click OK	Series Description	20D x 20H, 120 kVp/B-CBCTMF120
ient Orientation: Click below on feet to change patient entation (default direction is toes facing the doors).	Series Description	
	_	ТТШВ
		NWB
		FWB
		% Complete
rent Protocol		Start
ames kVp mA ms Multiple Pass		
361 120 5 12 no DoseAreaProduct CTDI		ок
803 mGy*cm*2 0.89 mGy		
UoseAreaProduct CTUL		
8.30 dGy*cm*2 0.89 mGy		-0
<- Back	Ready Xray Service Fault	Accept / Next ->

79

If any notes need to be added to go along with the current scan, they can be added in the Notes Field as shown below:

Patient Name	Procedure / Code	Protocol / Code
Johnson, Robert	CT LE LEFT WITHOUT CONTRAST/CTLELWO	20D x 20H, 120 kVp/B-CBCTMF120
ocedure Step		-17000
osition Patient In Scanner nd click OK		Series Description
ient Orientation: Click below on feet to change patient Intation (default direction is toes facing the doors).	Enter any notes here	Notes This is a follow up after surgery % Complete
rent Protocol ames KVp mA ms Multiple Pass 61 120 5 12 no IoseAreaProduct CTDI 830 d/Gy/cm^2 0.893 mGy		Start

Next, position the patient, using the instructions shown below.

Patient Positioning:


Before positioning the patient in the machine, remove his/her shoes/socks. We recommend the patient not step bare foot on the patient platform. Proper foot protection should be provided.

Have the patient put on FDA approved medical gloves and foot protection as recommended in Ch. 3 Safety Items, Patient Preparation Recommendations section.

Drape the patient with protective shielding for the procedure as recommended in Ch. 3 Safety Items, Radiation Safety section.

The patient will now need to be positioned in the machine. The Door Gates to the machine should now be in OPEN position in order for the patient to step in.

*Be sure to position your patient before clicking the OK button. Once the OK button is clicked, the Door gates will CLOSE.

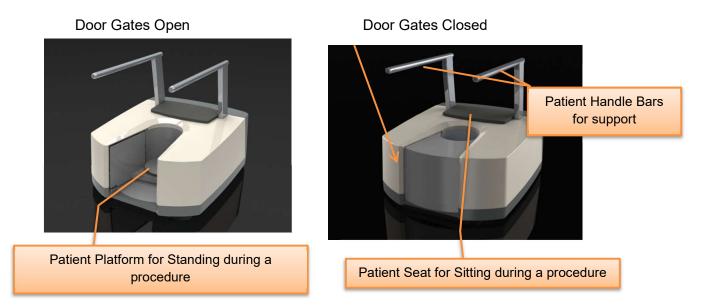

The patient should be instructed to step into the machine and position the feet on the platform. Also instruct the patient to use the handle bars for support as they step into the platform.

There are 2 standard positions for imaging the patient.

• <u>Standing:</u> for weight bearing images.

If Standing, the patient should step onto the platform and continue facing in the step in direction. However, the patient could also turn around and face outward if necessary. We recommend standing facing outward as it provides more clearance for the doors to close and is best for the patient to look at the operator for instructions.

Use the circular guides on the platform for feet position as described in the next section.

Note: Please remind the patient to stand in the appropriate weight bearing position and use the handle bars for stability during the scan. The handle bars are meant for support only.






• <u>Sitting:</u> if the patient cannot achieve standing position or if standing is not required.

If Seated, the patient should step onto the platform, turn around and face the doors and then sit on the padded seat on the machine. Use the circular guides on the platform for feet position as described in the next section.



Circular Positioning Guides:

These guides on the patient platform are intended to assist the operator in positioning the patient's feet/foot into the field of view.



The most <u>outer circle</u> is for the <u>Full, both feet procedure option (35 cm diameter)</u>. This is for a scan that needs to include both feet. Both feet should be positioned within this circle in order to capture both.


Positioning Illustrations are intended for Training purposes only.




Sample Results of Full both feet Field of View




The <u>second circle</u> is for the <u>Partial Single Scan option (20 cm diameter)</u>. This is for capturing one foot or a partial scan of one foot only. The area of interest for the scan should be positioned within this circle in order to capture it. So if you require the forefoot, then ensure that it is within the inner circle, however the hindfoot may not fit and would not be included in the scan (and vice versa). Smaller foot sizes may capture from Fore to Hindfoot.



Sample Results of Partial Single Foot Diameter Scan Field of View, Forefoot





Sample Results of Partial Single Foot Diameter Scan Field of View, Hindfoot




Alignment Light Positioning Guides:

There are 3 laser alignment lights to also assist the user in positioning the patient if needed. Access to turning these lights ON are on the upper corner of the left Door. When this button is pushed, the 3 lights will illuminate until the button is released.

One is a vertical light in the very center of rotation (center of the circles). The anatomy that this light falls on will be in the very center of the scan.

The other two lights are horizontal, one at the top of the scan (20 cm height), the other at the center of the scan (10 cm height).

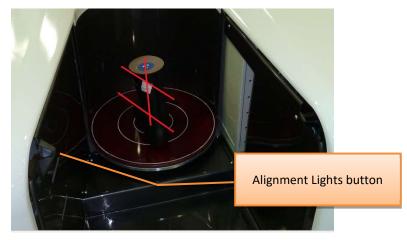


WARNING Laser beams can cause optical damage. The operator should avoid looking directly into the beams. The operator should instruct the patient to avoid looking directly into the beams. The use of optical instruments such as eyeglasses with large diopter or mirrors, increase eye hazard with this product.

Patient Instructions for a Scan:

Once the patient is properly positioned in the system, the operator should instruct the patient to **hold perfectly still for the duration of the scan**. It is very important for the patient to hold still. If the patient moves during the volume scans, the results may not be optimal. Data is being captured when the alarm is audible (and x-ray light is ON).

Once the patient is positioned in the machine, ensure the Patient Orientation is depicting the position of the patient. The suggested orientation is with the patients toes facing the door, feet depicted green in the image below. If the patient is standing with their toes facing the seat, click

on the green feet to change the Patient Orientation, when doing so, a pop up message will appear to confirm the choice to change the orientation as shown below:

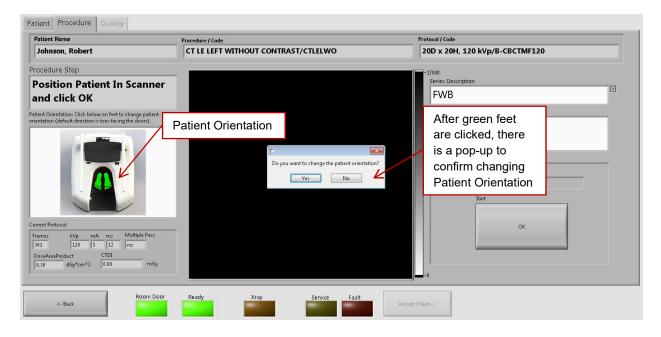

If "Yes" is selected to change the Patient Orientation, the feet will change position and turn yellow as in shown below:

Patient Name	Procedure / Code	Protocol / Code	
Johnson, Robert	CT LE LEFT WITHOUT CONTRAST/CTLELWO	20D x 20H, 120 kVp/B-CBCTMF120	
rocedure Step		-17000	
Position Patient In Scanner		Series Description	
and click OK		FWB	
tient Orientation: Click below on feet to change patient		Notes	
ment Protocol rames K/p mA ms Multiple Pass	Patient Orientation has been changed	% Complete Start OK	
361 120 5 12 no			
DoseAreaProduct CTDI 8.30 dGy*cm^2 0.89 mGy			


To change the Patient Orientation back again, click on the feet again and they will return to the original green feet in the default (feet facing door) position.

Next, click the OK button in the "Procedure" Tab in order for the Doors to close. Be mindful that the doors closing can result in a pinch point. Instruct the patient to be aware of this and keep all possible interferences clear.

WARNING Closing of the Gate doors creates a pinch point. Keep hands and feet clear when closing Gate


CT LE LEFT WITHOUT CONTRAST/CTLELWO	D	20D x 20H, 120 kVp/B-CBCTMF120
		J
	15	-17000
		Series Description FWB
		Notes This is a follow up after surgery
		% Complete
	Select OK to start scan	ок
		Select OK to

Next, a message will appear on screen instructing the operator to: "Press and HOLD Scan button".

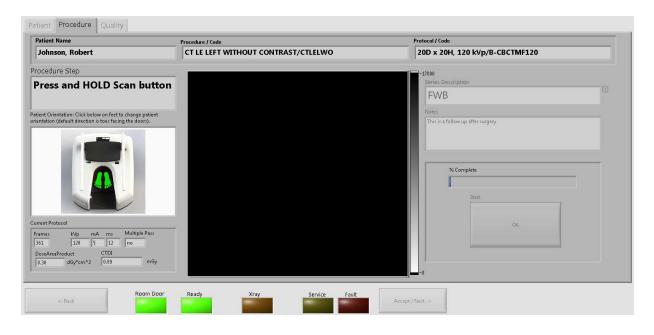


WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure.

The Scan Button to start the exposure is mounted on the Operator control box.

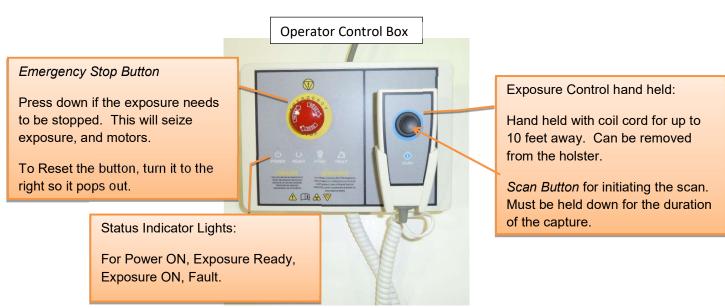

1. Deliver the Patient Scan Instructions to the patient.

2. Now Push & Hold the scan button down. During exposure an audible signal is generated by the machine, and the visual X-ray ON indicator lights will be illuminated in Amber color. The visual X-ray ON indicators are on the machine, the operator control box (above) and in PedCAT Acquisition "CB Scanning Device" software. The Operator should hold the exposure switch for the duration of the exposure as indicated by sound and lights.

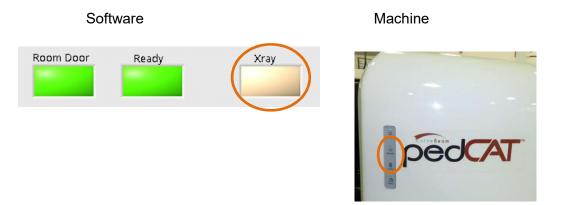

3. When the audible buzzer and "X-ray on" light turn off, it is OK to release the exposure switch.

NOTE: If you release the exposure switch before the exposure time has completed, the system will STOP exposing, however the gantry and motors will complete their sequence. If the button is released prematurely, the buzzer and indicator lights will turn off and the Error message below will display on screen:


an button Keleaseu	l During Scan	
ERROR: Scan Butto	n Released During Scan	

Emergency Stop: In the event of an emergency during a procedure (any moving component collides with any parts of the equipment or items in the environment, or that could cause physical injury to the Patient), the Operator or Patient should utilize one of the 2 the designated Emergency Stop buttons to turn off the power to the X-ray and all moving parts in order for the Patient to be safely removed from the machine. There is an Operator E-stop button on the Operator Control Box and there is a Patient E-Stop button on the machine by the seat. The Emergency Stop(s) when activated will remove ALL power from the machine. If the machine gates are closed, they will have to be opened manually and any obstructions to the patient exit will need to be manually removed before the patient is safely removed from the machine.





- 4. If performing a Large Field scan, the gantry will need to rotate around the patient twice. While the gantry repositions itself, the x-ray will not be fired and the scan button can be released. It is however critical that you inform the patient to not move and await the second pass with the x-ray. When the gantry is in position again, there will be a user prompt again to Press and HOLD the Scan button.
- 5. Once the capture is complete, the Door Gates will automatically OPEN. The patient can now safely EXIT the machine. If the scan is a Large Field of View scan, the machine will fire x-ray, reset itself, then fire again. The door will not open until all of the x-ray is completed.
 - If the patient is Standing, he/she should turn around while still on the platform, using the handle bars for support and step forward out of the machine.
 - If the patient is Sitting, instruct the patient to carefully stand and use the handle bars for support while stepping forward out of the machine.

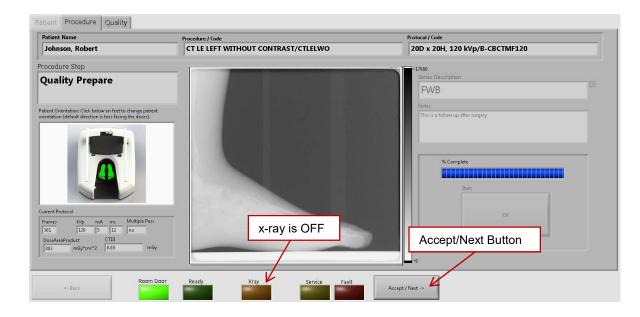


6. When the Accept/Next button becomes visible, click on it.

7. Once on the Quality screen, wait for all of the QA images to be present. Initially the QA screen will appear as in the following image.

Patient Name	Procedure / Code	Protocol / Code
Johnson, Robert	CT LE LEFT WITHOUT CONTRAST/CTLELWO	20D x 20H, 120 kVp/B-CBCTMF120
AX-FWB-FULL WC	Retrieved of the second	333 Axial 3 100 100 150 200 250 300 400 450 500 550 600
	Frame 0 25 50 75 100 125 150 175 200 225 250 275 300 325 3	666- -
<- Back	n Door Ready Xray Service Fault	Accept / Next ->

- 8. While waiting for the image to finish processing, check for movement of the patient during the scan, compare the first and last frames by using the "First/Last" button. View all images as they were acquired by using the slider below the raw frames or typing in a number to directly view that single frame.
- 9. Once the processing is completed, the right side of the screen will display the Axial slices. Scroll through them using the slider bar to the right of them.

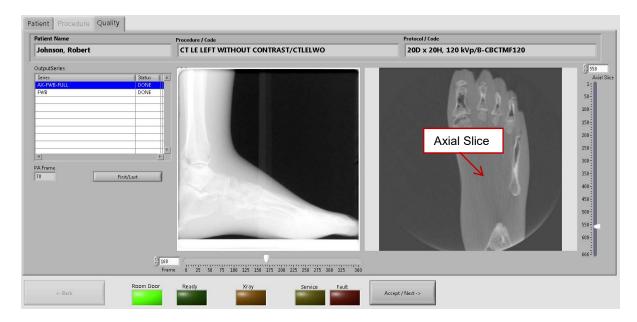

10. To view the dose report for this patient, click on the last line under Output Series. Some offices will have additional output series listed, as shown below, but the Dose Report is still the last entry in the Output Series List. The Dose Report will appear in the place where the Axial image was, as shown below:



11. Once certain the image looks like the anatomy desired was done so acceptably, click on the Accept/Next button.

NOTE: If there is any indication of vibration to the system, or malfunction to the system, or computer crash during a scan, please contact CurveBeam Technical Support for assistance. If there is a failed procedure, turn the machine off by the Emergency Stop button, following the below procedure.

Procedure for Emergency Removal of a Patient:

The system has undergone extensive testing of the mechanically, electrically and software performance, but if an unexpected occurrence is observed and/or the software locks up during a scan or an emergency arises where it becomes necessary to interrupt a scan and/or remove a patient from the system before a scan is completed, please follow these steps:

1. Press the EMERGENCY STOP button. This will halt the X-ray as well as the motors to the machine functions and all power to the machine. The message below will display on screen and will terminate the "CB Scanning Device" Acquisition software:



2. Open the Gate doors manually with your hands by using the slots at the top of each door to grasp and slide to an open position. Manually push the gantry out of the way if necessary.

3. Carefully assist the patient to step out of the scan platform area.

4. Reset the machine: Close the PedCAT Acquisition, "CB Scanning Device" software (if not already). Release the E-stop that was engaged by pressing in and turning the knob to the right until it pops up. Then turn the machine power back ON at the Main Circuit Breaker. Wait 2 minutes, then re-launch the PedCAT Acquisition "CB Scanning Device" software. Now the system can be operated again as expected

CHAPTER 7: Using the Viewing Software: CubeVue

Now that the data is acquired, it can be reviewed and post processed within the viewing software, CubeVue.

CubeVue can be accessed by the Viewing Terminal, MD workstation, or any computer that is connected to the PedCAT server via the facility network and has CubeVue software installed. Log into the Viewing Terminal, MD Workstation computer or any other workstation.



Then, to launch CubeVue, click on the CubeVue icon. The "About" Screen will appear showing software version & details. This can also be accessed by selecting *Settings/About*.



The CubeVue software has the following components to it:

- <u>Patient List:</u> for accessing, importing & exporting patient datasets.
- <u>Review:</u> for reviewing and processing the patient datasets.

PATIENT LIST:

When CubeVue is launched, the "Patient List" will display the list of patients with their datasets for the user to load. The volume datasets will display as Raw or Reconstructed. The Raw data sets are listed with the description of "RAW", the Reconstructed data sets are listed with the description being the protocol for which the scan was acquired.

🖤 CubeVue (c) 2011-2012 CurveBeam, L	LC Version 2.0.0.1		a di 💌
Patient List Review			
Load Import Print Hide Exp List List DIC	oort October 10 Date 9/1/2012 15 Name Date 9/1/2012 15 ID ••••••••••••••••••••••••••••••••••••		
Tools and Settings	Patient ID Patient Name	DOB - Study Date	Description
CLoad Option	Thomas-R922A2 Thomas, John	09/18/1984 09/01/2012 12:48 PM	Large Field (120 kVp)
	Brooks-3329 Brooks, Lauren	05/21/1978 09/01/2012 12:34 PM	Medium Field, Sharp Filter (120 kVp)
Load into 2nd work space	Brooks-3329 Brooks, Lauren	05/21/1978 09/01/2012 12:43 PM	Small Patient: Medium Field (100 kVp)
Show Optional Series	7877-09 Deacon, Jennifer	12/08/1963 09/01/2012 1:16 PM	Medium Field, Sharp Filter (120 kVp)
Raw	445-20993 Richards, Robyn	01/30/1950 09/01/2012 1:11 PM	Medium Field (120 kVp)
Screen Save			
Reformat			E
Show All			
			_
	4		
	L		
	<u>.</u>		
	dime.		T
			P
	Series # # of Images 1 1 RAW	Description *	
	1 1 RAW 2 1 Medium Field, Sharp Filter (120)	BA-3	
	z i Medium Field, Sharp Filter (120	күрј	
	Local Remote		

After selecting the patient name from the list at the top, then select which type of scan to view. The Show Optional Series allow the list to be expanded to show all types of scans, or limited to only show the scans that are checked. Typically the <u>Reconstructed</u> study will be the type of scan to select for viewing the dataset. Once the scan is selected, the Review Tab will be active.

If the patient that needs to be viewed does not exist in the patient list, it can be imported from an external location. The scan must have been taken using a PedCAT scanner in order to import



the patient scan. To Import a study from a PedCAT, select the Import Icon:

Once selected, a prompt will appear asking for DICOM Study or Raw File. DICOM Study would be the option to choose to navigate to the location of the study to import.


lease select type	e of import	23
Load DICOM st	udy (Yes) or Raw file (f	No)
	s No	Cancel



An Imported Study will reside in the "Local" Tab.

Type	Date	Mat
Recon	2/23/2012 10:50 AM	950 x 950

CubeVue allows for the user to have more than one scan loaded at the same time. This can be useful when comparing two scans done on the same person, a progression or a before and after type scenario. This is accomplished by first loading up a single scan. Then, from the Patient List tab (at the top), click first on "Load into 2nd work space" and then select the second series (scan) to open from the patient list.






Using the Series Layout tools: Series Layout the user can select which way to view the images, either both of the scans in a vertical mode (select 2x1) or a horizontal mode (select 1x2). The limit to the number of scans that can be opened at once is just two scans. To remove the scan and load a different second scan, close the series to be unloaded and then return to the Patient List. Repeat the steps above to load a different series into the 2nd workspace.

Conversely, if the patient's DICOM data needs to be sent to another location, the user can



Export the DICOM data. To do this, select the Export DICOM icon:

Once selected, the user can Browse and select the location to export the DICOM data.



To put the study on a CD, have a CD in the drive and then navigate to the CD drive as the destination folder for the Export DICOM. This will then place the DICOM data on the CD using the Windows Burning Software program.




There is a button that will allow the user to hide and unhide the Patient List. To do this, select the icon:



After 10 minutes of inactivity, the Patient List will be hidden for privacy purposes. In either case, when the list is purposely hidden or hidden after the 10 minutes, to unhide the Patient List, click on the Hide List icon to unhide the list.

It is possible to view only a subset of the entire Patient List. This can be helpful when a portion of their name or ID is known, or when trying to locate a patient that was scanned today, on a known date, or within the last few days.

To locate a patient in the list using a partial (or full) name or ID, start to type in the "Name" or "ID" fields. As information is typed in, the Patient List will start to decrease as only the patients that match the criteria entered are displayed. To do this, select the pulldown shown below to select a number of days since the scan was acquired.



Additionally, typing in a partial name or partial ID will display all the scans listed with the matching Name or ID as a part of the patient's information. Or, a specific date can be selected and all scans acquired on that date will be displayed. To select a specific date, click on the calendar next to "Select a date" in the image above.

REVIEW TAB:

Once the patient scan is selected from the Patient List, the scan will open in the Review Tab.

When the user opens a scan, there is a pop up box to select which anatomy is represented in the scan and appears as follows:




Select the appropriate check box that matches the anatomy represented in the dataset.


The Review Tab consists of 4 different Screens for viewing and processing data and a Main Menu Bar. The Tabs along the bottom are:

<u>Combined 3D/MPR</u>: contains a 3D rendering of the scan plus <u>multiplanar reconstructed slices</u>. <u>3D</u>: contains the 3D rendering of the scan only.

<u>MPR</u>: contains the multiplanar reconstructed slices only. Auto Built: contains the standard x-ray views.



Each "Plane" is color coded with Red, Green or Blue.

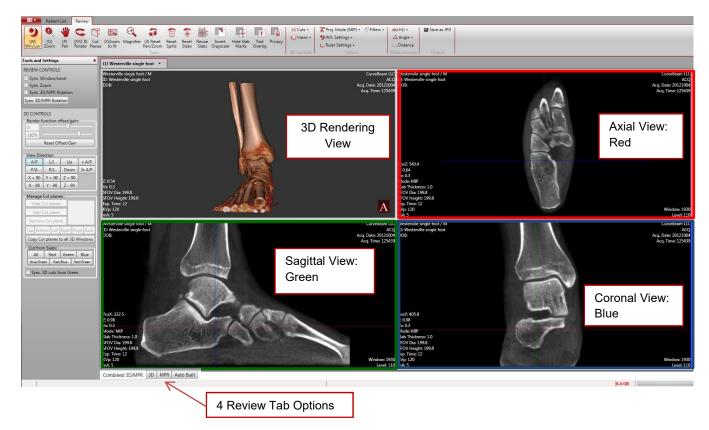


The Review Main Menu Bar (Ribbon):



Review Tab layouts.

MPR stands for Multiplanar Reconstruction. There are 3 views that are associated with MPR images. These views hold true for both the Combined 3D/MPR and the MPR Tabs: Axial, Coronal, Sagittal. Utilize the colored Slice Indicator Lines to know the slice locations.

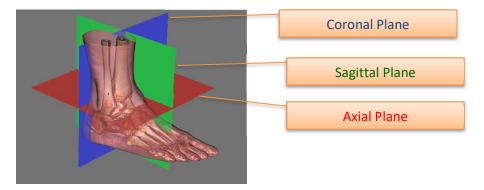

- **Axial:** slices through the anatomy from top to bottom, bottom to top: Red plane. <u>The "orientation of the image" is as if you were looking down on your foot/feet.</u>
- **Coronal:** slices through the anatomy from back to front, front to back. Blue plane. <u>The "orientation of the image" is as if you are looking at the foot/feet from behind.</u>
- Sagittal: lateral slices through the anatomy. Green plane.

Scrolling through cross section images in the MPR views:

The scrolling cursor is the Default cursor. \Box To scroll through slices, hover the mouse cursor over a desired view and this cursor should be enabled. Left Click, hold and drag to scroll through slices.

Alternately, each colored line in a Window can be clicked and dragged to scroll through its corresponding colored views.

The red line that cuts through two images, the Coronal and Sagittal, is the reference point for the Axial slice that is shown in the red outlined box. Moving the red line in either the Coronal or Sagittal views will change the slice location and the image displayed in the Axial view. The red reference markers will always depict the location of the Axial slice. This reference is the same for both the Coronal and Sagittal views as well, with the Coronal in green and the Sagittal in blue.

Alternately, for scrolling through slices in fine increments, when the cursor is hovered over an MPR image, use the mouse wheel to scroll through slices.



Each Tab has use of Universal Image Processing and Planning Tools:

K=X

Slab/Slice Thickness:

There are 2 methods to enable the tool for changing the thickness of the anatomy viewed, Hold down the SHIFT key and click on any of the colored reference lines and then drag the mouse to change the width of the line to represent either a larger or smaller slice of anatomy.


The cursor should change to this:

for horizontal lines or

for vertical lines.



OR, click on the "Resize Slabs" button on the Main Menu Bar. This will change the cursor for resizing. To disable the resize, click on the icon a second time and the cursor will change back to normal.

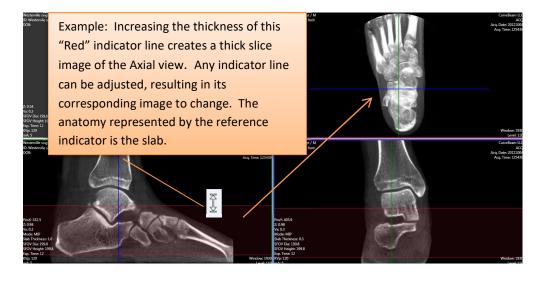

To move a Slab to a new location, click the now toggled "Move Slabs" Main Menu Bar and the cursor will change to its default $\iff \hat{1}$


reset. The message will appear as shown below:

which will allow you to "move" the slab to a new location by dragging the slab.

Menu Bar. If selected, a warning message will appear to verify that the slabs do need to be



button on the






Image Enhancement Tools: These are functions that can be used to enhance and manipulate the image for optimal viewing.

Window / Level (Brightness / Contrast):

To adjust the <u>Window/Level</u>, select the Win/Lev icon and then selecting a window to make the window/level change to. Changes are made by first clicking in the window, then moving the mouse up and down and then left and right until the optimal window/level is achieved. To deselect the Window/Level function, click on the Win/Lev icon a second time.

(W)Win/Lev



If the image does not appear as close as desired, then select the <u>Zoom</u> icon and select a window to change the zoom factor on. If you drag your mouse up, the image will zoom in and appear closer. As the mouse is moved down, the image will appear further away. To deselect the Zoom function, click on the Zoom icon a second time.




To adjust the image to a different location inside the window, the Pan function can be utilized. To center the section of the image desired in the window, select the <u>Pan</u> icon and then select the window to modify. Click on the image and hold the mouse down, while moving the mouse around and the image will move with the mouse movements. To deselect the Pan function, click on the Pan icon a second time.

æ	
Magnifier	- 200

Image Magnifier:

The Magnifier icon will provide a magnification of the selected image. When the mouse is moved around the anatomy in the selected image box, the magnification box will be continually updated with the new location of the mouse.

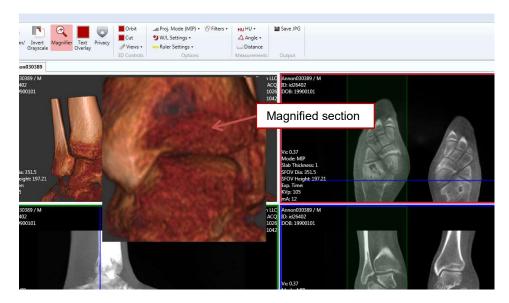



Reset Pan/Zoom:

Once the Pan and Zoom functions have been used and a different section of the anatomy is of importance, then the user can begin the Pan and Zoom process again by selecting the Reset Pan/Zoom icon. When the Reset Pan/Zoom icon is selected, the image will appear as it did when the study was originally first loaded.



Splits / Reset Splits: 1

The individual windows can also be moved to allow for a larger window for any of the four windows. So that if the user would like to see a full screen of the Axial image, mouse click on the center of the four windows and adjust the window sizes so that the Axial image takes up the majority of the window.




Once done with viewing the Axial window, the window sizes can be reset with the use of the Reset Splits icon. This icon will put the windows back into the configuration they were in when the software scan was freshly opened.



Invert Grayscale:

The Invert Grayscale icon will invert the grayscale on all the images, except the 3D image. Click the Invert Grayscale icon again to revert back to normal grayscale.

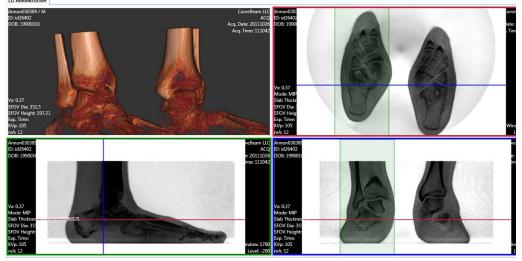

Text Overlay and Privacy:

The overlay on the images is most of the informative text on the image. If the user does not want to display the information, there are two options available. The Privacy icon:



will remove ALL patient information from the image other than Patient ID#. This can be useful if the desire is to maintain a level of anonymity when viewing the scan on the screen. The image should NOT be printed when the Privacy icon is selected and no patient data is displayed. To allow for the basic patient information, then the Text



Overlay icon should be selected. Text Overlay This allows the user to display some information but also remove the excess information from the Image Windows.

Projection Mode:

There are 2 options available for projection mode, one is "Radiographic", the second is "MIP". Radiographic is the image displayed as a normal radiograph.

MIP stands for Maximum Intensity Projection. This is an image tool that is only usefull for thick slice slabs. It will display for each pixel, the most dense valued pixel in the depth of the selected slab, which means it will display the brightest pixel (voxel). Below is a comparison of a thick slice slab as a Radiographic projection vs. an MIP projection.



Radiograph

MIP


To alternate between Radiograph and MIP, click the Proj. Mode icon. It will display to

you which mode it is currently toggled to.



Filters:

There are 3 filter options available; Smooth, Normal, Sharp. Filters can be applied to enhance images. The default filter type will be Normal. But if the image requires a little more detail, than the Sharp filter can be selected. Smooth will make the edges of the images appear more smooth, but may lose some detail. Filters are often a personal preference. Select the Filters icon to apply one of the 3 options.




Measurements: There are various measuring tools for treatment planning. <u>HU:</u> These are for measuring Hounsfield Units, which is density value of an area of interest.


Angle: These are for measuring angles on the anatomy of interest.

<u>Distance:</u> This is for measuring distances in millimeters. There is also a Ruler that can be displayed on the images to assist in quick visual reference of length.

HU Measurements: The HU tool has a drop down with 6 options; rectangle, circle, freehand and line for general use and then QA set Small and QA set Large for doing the QA procedures.

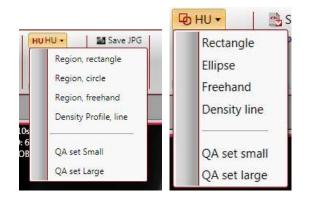


Any of the general use regions can be selected for creating a region of interest (ROI) on the bone in order to obtain a density value reading. For example, if "Ellipse" is selected, an elliptical ROI can be drawn by point click and drag. Then click a final time to anchor the ROI. The measurement reading will display in the upper right hand corner of the image window. A maximum of 10 measurements can be made in one image window. This tool will remain enabled until disabled by clicking the selection again.

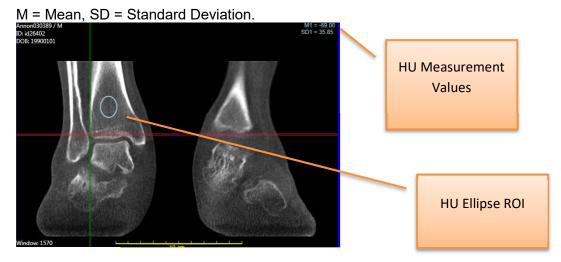

Follow these instructions for the rectangle or freehand as well.

The Density Profile line displays in graphical form. Draw a line and the graph will appear.




For doing the QA procedures, there are two sets of pre-sized HU regions. Selecting the "QA set Small" will draw small circles that are used to determine the HU of the various


materials on the QA Line Pair Phantom. The "QA set Large" will draw large circles that are used to determin the HU of the water.

Angle Measurements:


The angle tool has a drop down with 4 options for measuring angles; Simple, Prepare Cobb, Cobb, and Correlate Cobb:




<u>Simple Angle:</u> Select "Simple" to enable the Simple angle tool. The Simple Angle has 3 points of reference. Point, click, move, click, move, click to finish (3 clicks). This will result in an angle in degrees, and the measurement will display in the upper right hand corner of the window. A maximum of 4 measurements can be made in one image window. This tool will remain enabled until disabled by clicking the selection again.

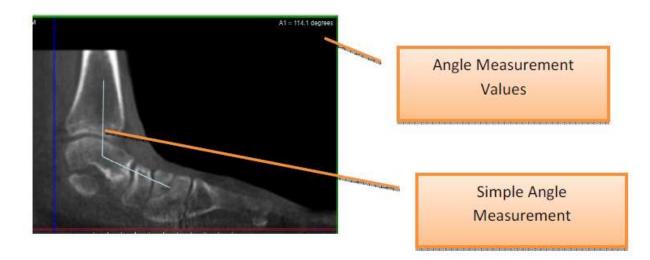

<u>Cobb Angle</u>: First select "Prepare Cobb" to orient the feet properly. Then select "Cobb" to enable the Cobb angle Tool. The Cobb angle requires creating 2 separate lines and the tool will calculate the angle at the point of "intersection" of those 2 lines:

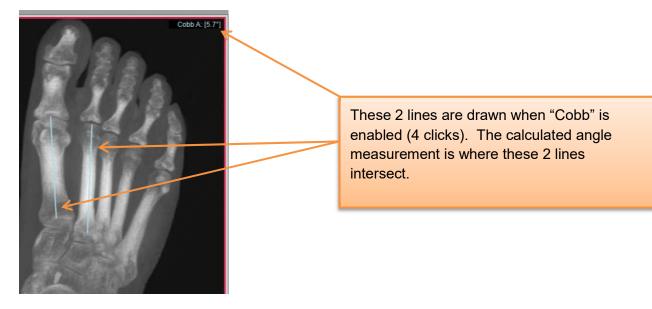


Correlate Cobb Angle: Create 2 sets of "Cobb" lines and then select "Correlate Cobb" to calculate and angle where the 2 yellow dotted lines intersect:

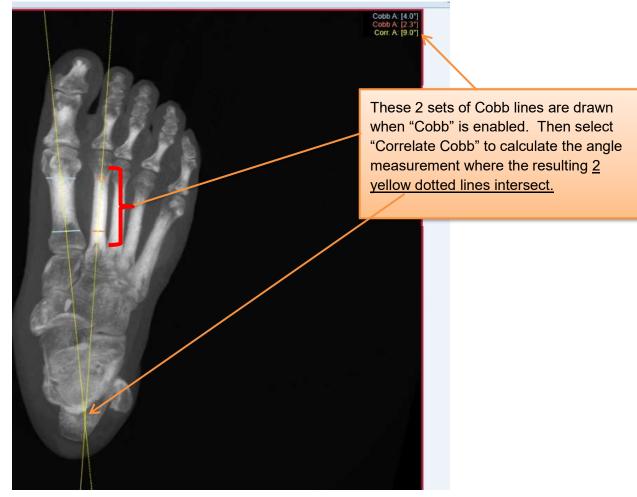


Distance Measurements:

Select the Distance Tool icon to enable the distance tool. Distance has 2 points of reference. Point, click, drag, release to create a line. This will result in length measurement in millimeters, and the measurement will display in the upper right hand corner of the window. A maximum of 10 measurements can be made in one image window. This tool will remain enabled until disabled by clicking the selection again.

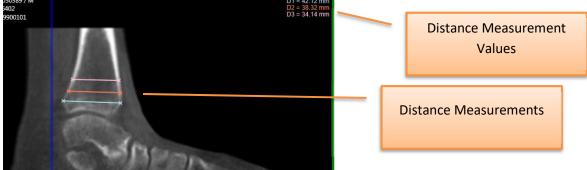

Removing Measurements:

All measurements can be removed by hovering over the values in the corner and right clicking on them. This will display a pop up window. Select either Remove measurement which will remove the last one drawn on or Remove all measurements which will remove all from both the corner and the illustration on the image.



Ruler Settings:


Also Note that there is a Ruler Tool that can be displayed on the bottom of the image window for quick distance measurements. This overlay can be enabled or disabled by clicking on the "Ruler Settings" icon. Click Show Ruler to display the yellow ruler at the bottom of the image window.



Ruler Settings -

MPR Tab:


The MPR Tab has the 3 MPR views and no 3D Rendering. Two additional tools are available only within the MPR Tab, they are the "MPR Cut" tool and the "MPR Explorer" tool. These tools are only enabled when you are on the MPR Tab and are in the "Options" area.




When MPR Cut is selected, the cursor allows the user to draw a "cut line" on any of the 3 MPR images in order to display a customized slice in any direction in the lower right hand corner window.

After selecting MPR Cut, click anywhere in an image to start the MPR Cut Line. The cut line can be straight or curved. For a straight cut line, click in 2 spots, then double click to complete the sequence. For a curved cut line, make multiple clicks in a curved direction.

MPR Straight Cut Plane: Created in the Axial view. The resulting cut displays in the lower right corner.

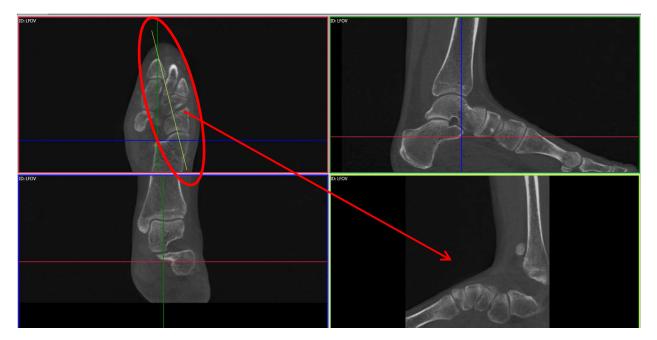


MPR Curved Cut Plane: Created in the sagittal view. The resulting cut displays in the lower right corner.

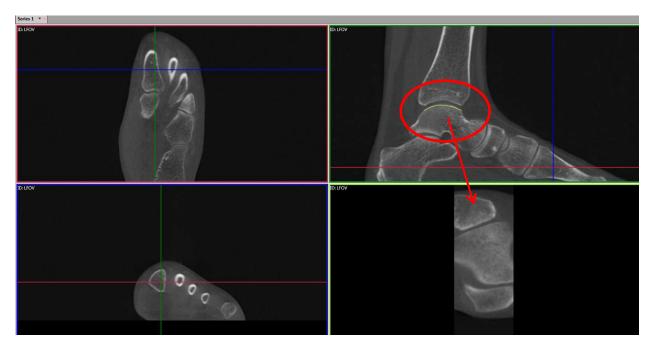

When the MPR Explorer is selected, the cursor allows the user to create the MPR Explorer tool on any of the 3 MPR images in order to rotate around a center point with the image displayed in the lower right hand corner window.


After selecting MPR Explorer, click anywhere in an image to start the MPR Explorer, which will appear as follows:

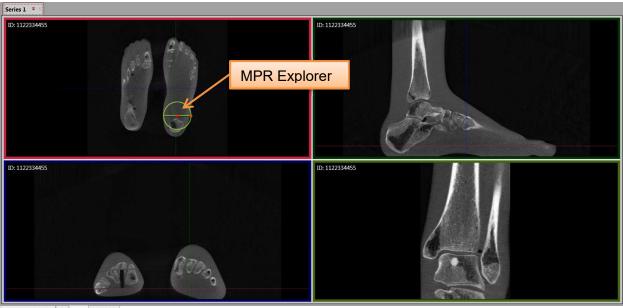

Combined 3D/MPR 3D MPR Auto Built

This tool can be moved around the image by clicking on the center red dot and dragging the tool to the desired location. To expand the area displayed, click on the red dot on the outer edge of the circle and drag the dot for either a larger or smaller region to view using the tool. Also use the red dot on the outer edge of the circle to rotate it around to view different images in the lower right window. The image shown will correspond to the green line drawn through the circle, so as the red dot is moved around the circle, the image in the lower right hand corner will adjust accordingly.


Drag center red dot to move Explorer tool to different locations within the window



Drag this red dot in or out to contract or expand the circle.

Rotate it to view a different section of anatomy.

Right click on the center green line, with the cursor that points up, to get the following options:

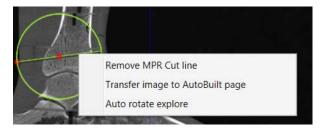


The "Remove MPR Cut line" will remove the MPR Explorer tool from the image. This allows the tool to be placed in a different window if desired. The "Transfer image to AutoBuilt page" will transfer the image the tool is on to the Auto Built tab. To have the image represented by the tool, the image in the lower right hand window, moved to the Auto Built tab, right click on that image and select to move it from there. To allow the image to rotate freely without needing to manually rotate it, select the "Auto rotate explore" option. Right clicking on the outside of the circle will do all the same options except it will not allow for the auto rotate option.

To use the MPR Explorer tool in a different MPR window, such as changing from axial to sagittal window, delete the tool from the axial window and redraw it in the sagittal window.

Print Images


A Print option appears as an Output function along the top menus.




To use click on Print and then select either "Print Image" or "Print All Images". If Print Image is selected, the currently active image will be the one printed.

Auto Built Tab:

The Auto Built tab is used to display the standard x-ray views as shown below:

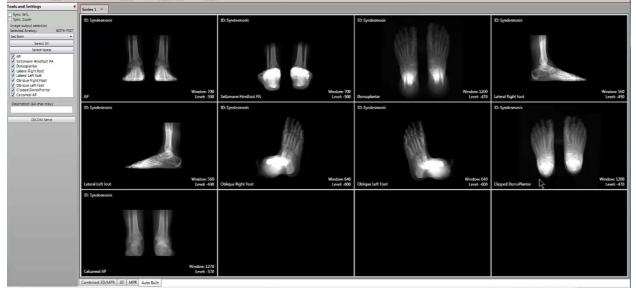

When the scan is just of a single foot, fewer images will appear. In order to show only certain images, the checkboxes, unchecked images will not be shown. The Tools and Settings selection for the Auto Built tab is shown below:

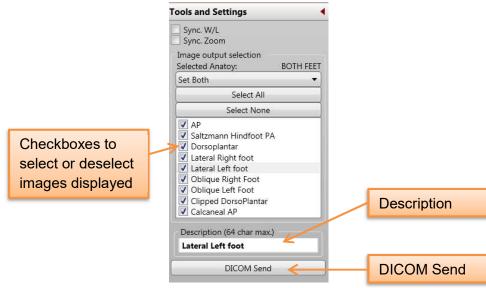

The Description field in the above image depicts the description given for the selected image and can be changed as desired. Just type in the field and the corresponding image will have the description updated.

All images shown can be double clicked on to view the image full screen. All of the usual measurement and navigation functions, such as Pan, Zoom, etc are still accessable.

When the DICOM Send button is selected, the DICOM Sender box will be displayed. In this window, one or multiple **Destinations** for the data send can be configured. Configure a Destination with the appropriate data and click the **Update** button to Save. To add another Destination, click on **New** and edit the Destination items, click Update to Save. Once there are Destination(s) configured, they will remain in the list unless deleted.

		DIC	COM Sender
Destination			New: to configure one or more additional Destina
Name :	Default		
Host :	localhost		Update: to Save a New Destination
Port :	11112		Delete: to delete a highlighted Destination
Local AE :	CUBEVUE		Delete: to delete a highlighted Destination
Remote AE:	PEDCAT	New Update	Delete
	10-10-10-10-10-10-10-10-10-10-10-10-10-1		
	After successfu	al send also save the output locally	·
Progress	After successfu	Il send also save the output locally	
Progress Status Read		il send also save the output locally	
		il send also save the output locally	

Click **Start** to begin the Send. The Send time will depend on how many datasets and destinations are selected, the number of reformats created, and the speed of the PACS network. When the Send is completed, the Status will read "Completed".

Any of the non-3D images thoughout the software can also be added to the Auto Built tab by right clicking on them.

Tools and Settings Panel:

REVIEW CONTROLS:

<u>Sync Window/Level:</u> when this item is "checked", any Window/Level adjustment to an MPR image will make the same adjustment to the other MPR images.

<u>Sync. Zoom:</u> when this item is "checked", any Zoom adjustment to an MPR image will make the same Zoom adjustment to the other MPR images.

<u>Sync 3D/MPR Rotation</u>: When this item is "checked", any rotation of the 3D rendering will also rotate all 3 MPR images to the same angle.

<u>Sync 3D/MPR Rotation button</u>: When this button is clicked on, the MPR images will snap to the rotation angle of the current 3D rendering rotation.

Tools and Settings	4
REVIEW CONTROLS	
Sync. Window/Level	
Sync. Zoom	
Sync. 3D/MPR Rotation	
Sync. 3D/MPR Rotation	


3D/MPR Rotation, (Volume Rotation, Volume Tilt):

The default image planes of MPR views are as the scan was taken. However, if you wish to rotate or tilt the MPR images to different planes, this can be achieved using the 3D rendering and the Sync 3D/MPR functionality.

Below is an example.

If this is the starting view below and then 3D image was tilted upwards either with the Sync 3D/MPR Rotation or by clicking the button after the rotation, then the MPR rotation will change from picture A to picture B:

Picture A: the 3D rendering is in an A/P direction.

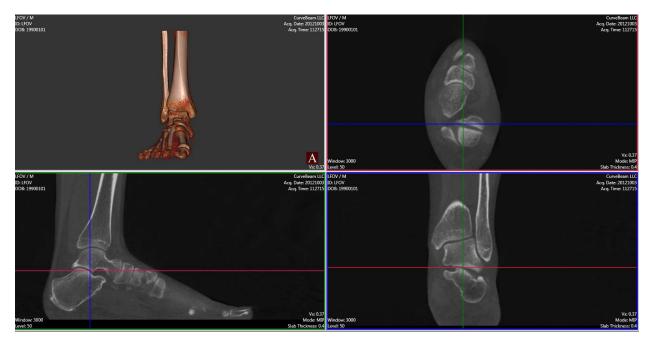

Picture B: The 3D rendering has been rotated with the toes up slightly. Observe how the upward tilt of the 3D rendering is now reflected in the MPR views. The first metatarsal is now on the same horizontal plane.



For fine control of the X, Y and Z rotations of the 3D rendering, press the associated keyboard letter and HOLD while rotating the 3D image.





X key: Hold the key down and move the mouse up or down on the 3D rendering. This will tilt the rendering in an even up / down plane.



Y key: Hold the key down and move the mouse left or right on the 3D rendering. This will tilt the rendering in an even side to side plane.






Z key: Hold the key down and move the mouse in an up or down direction and this will move the 3D rendering clockwise or counterclockwise.



3D Renderings:

The 3D Rendering image displays in both the Combined 3D/MPR Tab and the 3D Tab. The combined allows the user to scroll through MPR slices for Viewing/Planning as well as edit and manipulate 3D renderings. The 3D Tab only displays the 3D renderings. However, the 3D Tools are similar for each.

Combined 3D/MPR Tab:

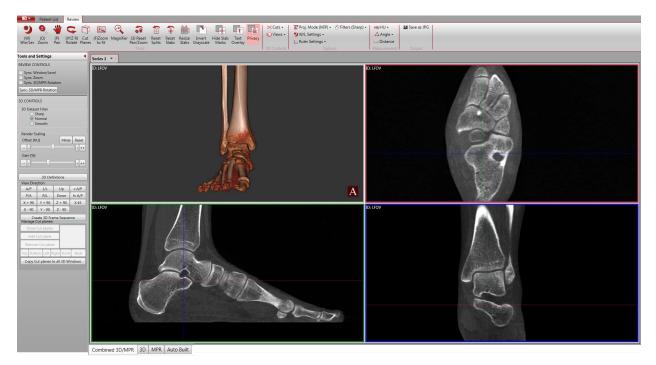

3D Tab:



The Zoom, Pan & Rotate buttons on the Main Menu Bar all can be activated and used in the 3D Rendering window.



3D CONTROLS: the 3D CONTROLS within the Tools and Settings panel contains most of the 3D rendering functions.

<u>3D Controls – Filter:</u> Use the filters to adjust the image.

3D CONTROLS	
3D Dataset Filter	
Sharp	
🔘 Normal	
Smooth	


The Sharp selection will display the full resolution dataset.

The Normal selection will display the 2x2x2 resampled dataset.

The Smooth selection will display a smoothly filtered 2x2x2 resampled dataset. When first opening a patient scan, it will be depicted as Normal. When the selection is changed, it will be changed for all screen layouts, ie in Combined as well as 3D screen layouts.

<u>Render Function offset/gain:</u> These tools adjust the thresholding for the 3D rendering.

Drag the slide bar to adjust from soft tissue to bone and vice versa. To reset both back to zero, click the Reset Offset/Gain button.

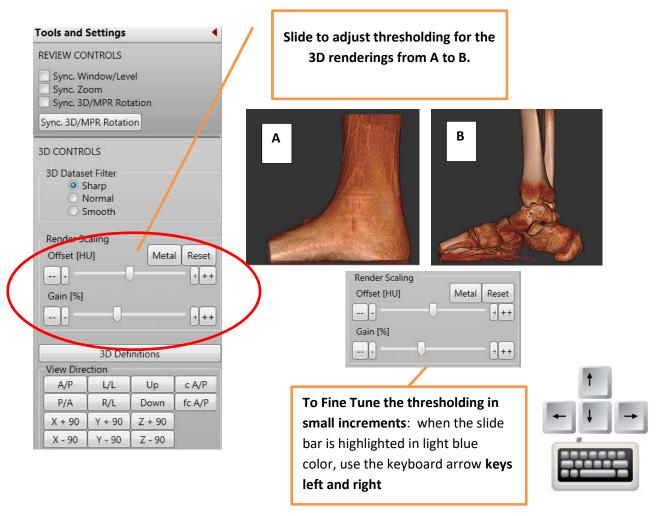

The Render Scaling sliders have a Metal and Reset button for Offset and Gain. The Metal button can be used if the study is loaded for the first time and nothing but a piece of metal (screws, etc) is visible. Only click on the button **once**. Clicking on it repeatedly will apply the scaling multiple times and the render ranges will become useless. If this does occur, click on the Reset button to reset the image to the original render.


Offset [HU]	Metal	Reset
	0	+++
Gain [%]		
		- 00.

To make fine tweaks to the Offset and Gain, adjust using the sliders. The sliders will produce relative render scale changes, which means after the slider is adjusted, it will return to its "home" position. This allows for HU range coverage scaling, meaning a larger range is achievable in the small slider. After coarsely adjusting the sliders (Offset is recommended over Gain), then use the buttons on the ends of the sliders (--/-/+/++) for fine adjustment. Click on the buttons to the left or right of the slider then use left and right arrow keys on the keyboard also for fine adjustment.

3D Definitions

A way to edit the transfer function has been added, allowing the user the ability to create a new render type. The process is started by clicking on the "3D Definitions" button under Tools and Settings.

3D Definitions	

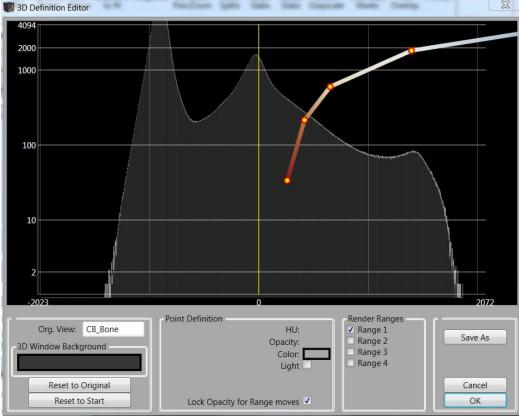


The 3D Definitions button will bring up the following 3D Definitions Editor window:

The 3D Definition Editor, also called Transfer Function Editor (TFE), once opened, shows the current volumes' histogram along with some control points and a colored render line connecting them. The continuous connection from a very left to a very right control point is called a render range, and there can be multiple render ranges. These render ranges must not overlap. If they do you will get a red "collision" indication, sign for you to move a render range out of the way. The rendering of colliding render ranges is undefined and may give you unexpected results. The changes made in this TFE will be visible in the 3D window. It may help to adjust the location of the Editor window so that the 3D image is also visible when the Editor is being used.

To adjust the render line, hover over a point for the plus icon to move the single point. Hover over the line for the hand icon to move the entire line left and right. To adjust the Offset and Gain for the range, use the sliders under the Tools and Settings menu. It can be desirable to move the ranges with the sliders for different scans as the HU value can fluctuate from scan to scan.


The points on the graph can be moved by left clicking on the point and adjusting it. Also a right click on the point will allow the user to remove the point, remove all points, or change the color of the render. It is also possible to adjust the range, but making adjustments using the Tools and Settings slider allows for easier adjustments. To add a point, right click on the line where the new point is desired to add a point.

To adjust the color of the render, either left click on a point, then select the color box from the Point Definition section below. Or, right click on the point to change the color. See the image below for locations.

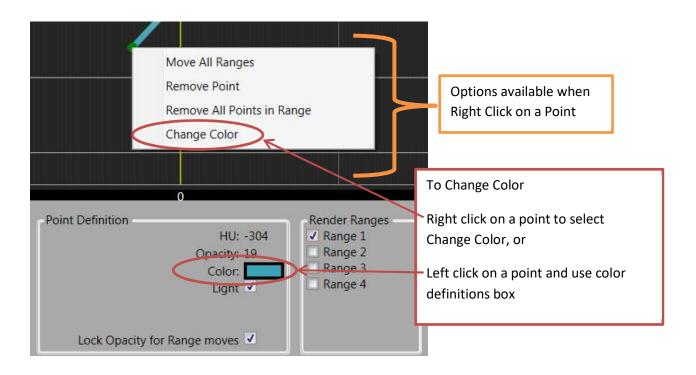


When adjusting the render range, the active range has the point that is solid green. The green point's values are listed in the Point Definition box, displaying the HU, Opacity, Color, and Light source. Use the Light check box to turn on/off a light source associated with that selected/green point.


When the 3D Definition Editor starts, only 1 range is shown. To add additional Render Ranges, select the check boxes for additional ranges. There is a limit of 4 render ranges. The image below shows a second render range was just selected. The points for the new range appear at the top right.

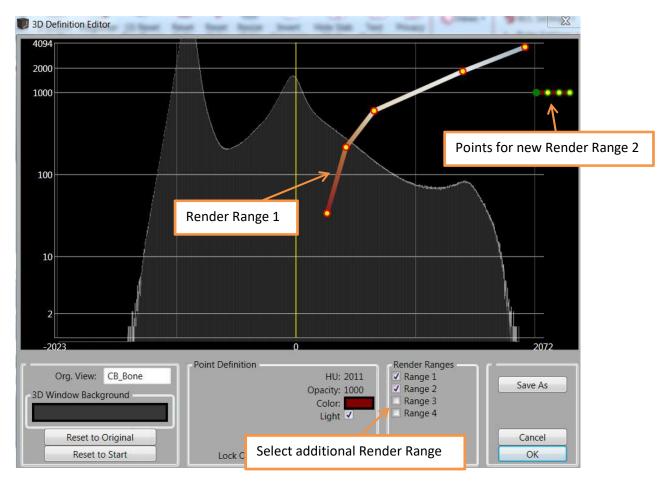

Each point in the new render range can be moved, but each new render section cannot cross another render section. None of the points of this second render section will be allowed left of any of the points from the first render line. If moving a single point, a red line will appear and not allow the render sections to cross into each other's range. If moving an entire render range into another render range section, a red zone will appear. Adjust the two sections so that they are not overlapping each other. The image below shows what will appear if the sections do cross over each other.

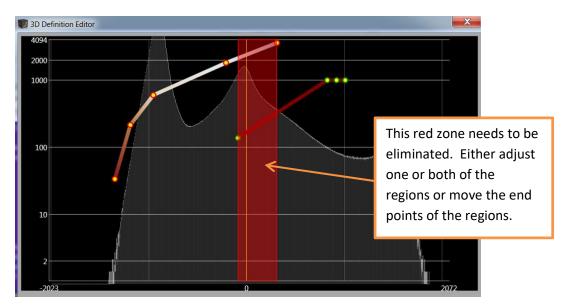

The background color of the 3D window can be adjusted by selecting a new color under "3D Window Background". Click on the color box to change the color. The 3D window will update after the selection is made.

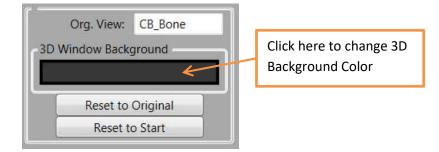

The underlying default render type is listed in the "Org. View" box – in the above it is "CB_Bone". The "Reset to Original" button can be used to reset back to the default render type listed in the "Org. View" Once completed with the changes to the render type, if you wish to save the changes, click on the "Save As" button in the lower right corner of the 3D Definition Editor (TFE). Maintain the default directory that appear with the Save As button. Provide a unique name so that it can be used with other scans in the future. The new render types created with this method will be available to select from under the Views -> Render Type. Once done with the 3D Definition Editor (TFE), select OK to maintain the changes to the current dataset.

View Directions:

A/P	L/L	Up	c A/P
P/A	R/L	Down	fc A/P
X + 90	Y + 90	Z + 90	
X - 90	Y - 90	Z - 90	

There are automatic snap to View Directions for a quick rotation of the Rendering to a desired view:

View Dire	ections
A/P (Anterior / Posterior):	Up (looking up into bottom of foot/feet):
P/A (Posterior / Anterior):	Down (looking down onto top of foot):
L/L (Left Lateral):	C A/P (Conventional Anterior / Posterior): down, 15 degrees from vertical.
R/R (Right Lateral):	

<u>Cut Planes:</u> To cut a 3D rendering from an entire plane, first click the **Cut Planes** icon from the Main Menu Bar to activate the functionality.




Once enabled, a cut plane is placed within the center of the 3D Rendering. Also, the "Manage Cut Planes" tools will be enabled in the 3D Tools area.



Original Rendering

After clicking on **Cut plane** icon. A cut plane will Auto drop into the center of the volume and cut out half the 3D rendering. *Manage Cut Plane Tools* will also be enabled.

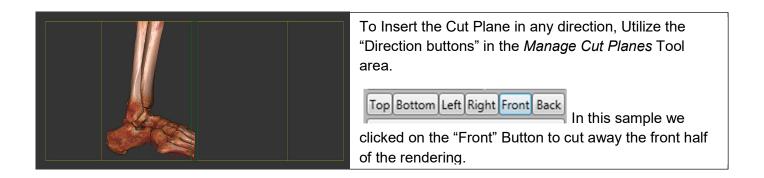



NOTE: The angle of direction of the cut plane can be adjusted to any angle by holding down the CTRL key and dragging the mouse in any direction.





Peeling Away the rendering:

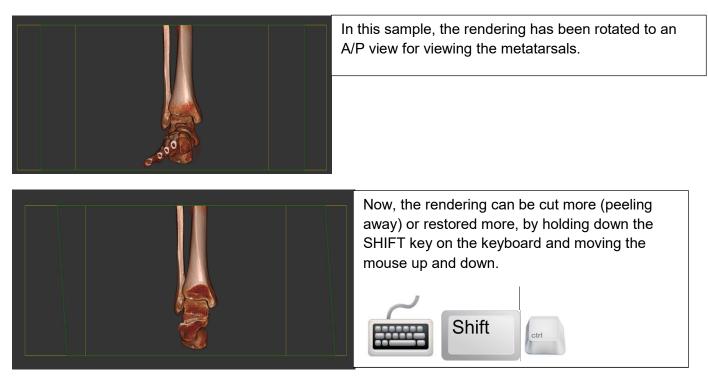

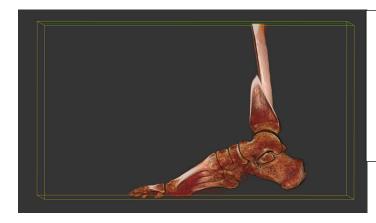

This cut plane was rotated to a sagittal plane by clicking the "Left" button to cut through the foot from the medial side.

Top Bottom Left Right Front Back


Multiple Cut Planes can be inserted and manipulated by clicking on "Add Cut Plane" button. To Remove Cut Planes, highlight the Plane in the list (Plane 1, Plane 2, Plane 3....) & click on the "Remove Cut Plane" button. To Hide a Cut Plane, highlight that Plane in the list and click on the "Hide Cut Plane" button.

Hide Cut planes	Plane 1
Add Cut plane	Plane 2 Plane 3
Remove Cut plane	Plane 4
Top Bottom Left Rig	ht Front Back

If desired, to transfer the 3D Rendering that was just designed to the other 3D Window click on the "Transfer Cut Planes to all 3D Windows" button. Otherwise, the other 3D window will be a fresh rendering.

Cut From Slabs:

Another method of cutting a 3D Rendering is to "Cut From Slabs". In order to Cut from Slabs, you must first create Slabs in the MPR image(s). Then use the "Cut From Slab" Buttons to make the cut(s) on the 3D image.

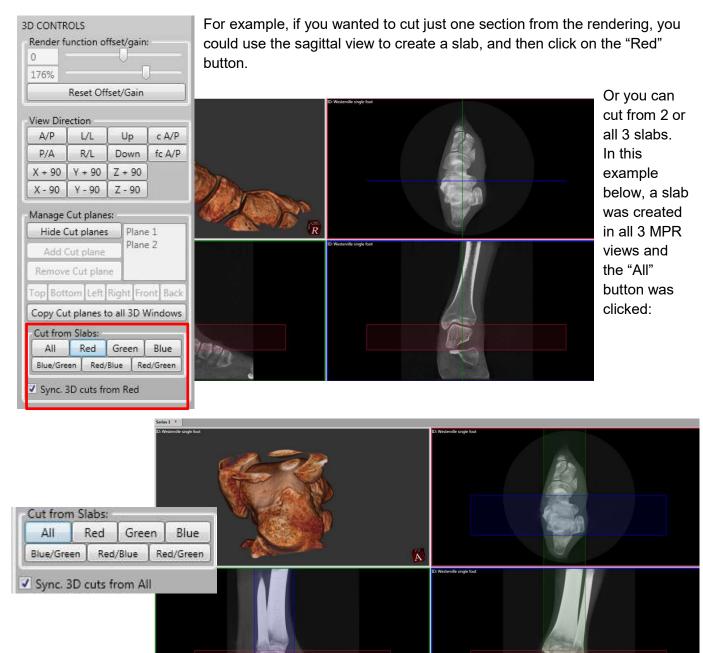

Note: to restore the original 3D rendering, click on the "Hide Cut Planes" button under Manage Cut Planes.


ender Types:

To select various 3D Rendering types, click on the Views icons in the 3D Control area. This will display a pop up window with various options to select from. Select Render Type.

Views • Ru	ler Settings •
Render Type	1
Full Convention	nal A/P
Conventional A	VP
A/P	
P/A	
Left Lateral	
Right Lateral	
Up	
Down	
	Render Type Full Convention Conventional A A/P P/A Left Lateral Right Lateral Up

When Render Type is selected, a window will display thumbnails of the various default types of 3D renderings currently available. They are:

- 1. bone_skin
- 2. bone_skin2
- 3. bone_transparent skin
- 4. transparent_colorized
- 5. x-ray

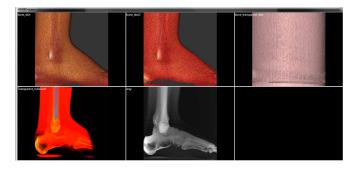

When one of these options is selected, that render type will display in the 3D Render window. Now you can adjust the rendering by using the Render function tools and dragging the slide bars. The most effective change of renderings will come from the slide bar.

Creating 3D Frame Sequences:

There is the ability to create a WMV video or frame sequence of the 3D image rotating around either the X, Y, or Z axis. To do this, select the Combined 3D/MPR screen at the bottom of the screen as shown below:

ick vs	KVp: 120 mA: 5	Select Combined 3D/MPR Tab
	Combined 3D/MPR 3D MPR Auto Bu	uilt

Then under the Tools and Settings on the left side of the screen, select the Create 3D Frame Sequence button:

	IV L	Down	
X + 90	Y + 90	Z + 90	X 45
X - 90	Y - 90	Z - 90	
		me Seque	nce
Manage (Jut planes.		
	Cut planes		

Select Combined 3D/MPR Tab

A pop up window as shown below will appear that allows for the selection of which axis to rotate around, how to save the output and how many frames to use to c. For each of the different output selections, the pop up window will look slightly different to ask the user to provide a location to save the video.

DM e to patient folder e to custom location
to patient folder 36
to custom location

Under the Direction heading, select the axis to rotate around, either X, Y, or Z axis.

Under Output, select where to output the video that will be created.

- If **DICOM** is selected, A new DICOM series is created and is automatically saved on the Local tab under file type "screen". If the "send after saved" box is checked, the new DICOM series will also be automatically sent to selected the DICOM destination, found on the DICOM Destination tab. This DICOM destination can be user-configured.
- If **Save to patient folder** is selected, the video (.wmv file, not DICOM series) will be saved locally (your computer C:/) but will not be visible in the Patient List. This option is NOT recemmended.
- If **Save to custom location** is selected, the location will need to be entered in the field below, or the Browse can be used to set the location. A .wmv file will be created and saved at the specified location.


The Number of Frames value represents how many total frames or images that will comprise the video and can be adjusted as desired. For example, in DICOM, 360 degrees rotation divided by an entry of 36 Frames means you will create a series of 36 images, each one appearing to advance approximately 10 degrees in rotation from the preceding frame. The other two output results in the creation of a Windows Media audio/Video file (.wmv) which requires using a video player to view.

The Frame Rate shows how many frames will be displayed in Frames Per Second when the video is viewed.

Once all of the fields are set to the desired values, click on Start to create and save the video.


Saving Sessions and "Series" Tab Functions:

When a study is loaded, the Patient Series Tab will display that current study name. The dataset can also be closed or "unloaded" from this tab by clicking on the " \mathbf{x} " in the corner. The session work that has already been completed will be auto saved, so when the study dataset us re-loaded again, the sessions work will automatically load.

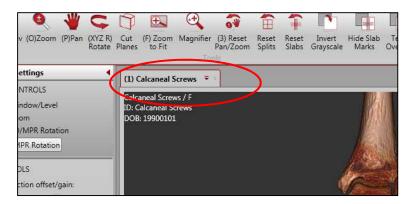

However, there is also a Drop Down Menu that provides a "Save Session" functionality so that you can save several different planning's.

Click the Drop Down Icon to access the Drop Down Menu to Save Session:



From this menu, then select "Save As a New Session" for the Session Manager Dialog Box. Enter in an appropriate Session Name over the "Type a Description" Session Description. Click inside this text box to enable the cursor for typing. Click OK to close the Session Manager.

ocosionis ma	nager			x
Patient nam	e:	Patient ID:		Patient date of birth:
Calcaneal Sc	rews	Calcaneal Screws	19900101	
Session ID	Creation Date	Description		
	2012-12-05-08:35	i:12 Auto-generated		
1	2012-12-05 08:35	i:38 Type a description		

Then at any time, a Saved Session can be accessed and loaded by selecting "Load Session" from the Drop Down Menu. This will open the Session Manager where you can then highlight the desired Session and click OK to load.

(1) Calcan	neal Screws 🔻	c			
18005	Screws / F	Load Session			
ID: Calcane		Save Session			
DOB: 1990	00101	Save As New Session			
		Reset Session			
		Unload Study			
		Unload Both Studies			
		Swap Studies			
		Split Study			
Sessions Mar	nager				
Patient name	N22	Patient ID:			ate of birth:
Calcaneal Sc	crews	Carcaneal Screws		19900101	
Session ID	Creation Date	Description			
	2012-12-05 08:35:12				_
1	2012-12-05 08:35:38	Treatment Plan			
Select a Ses	ssion to load		Delete	ОК	Cancel

From the Drop Down menu, the Dataset Study can also be Reset, which will re-load the original dataset to its pre-worked state. And a Dataset Study can also be "unloaded" from this drop down menu as well.

Input: Load Function

The Load function is provided to allow the scan to be viewed in CubeVue, either the Raw or Recon file. But, when using the Load function, the patients scan will NOT be added to the existing Patient List. Any changes to the scan that are made, measurements, etc, will not be saved. The scan will not be added to the database of scans available to view.

To perform the Load function, click on the Load icon from the Patient List tab:



Then follow the steps to load the study into temporary memory for CubeVue. Remember, any plannings done will not be saved.

Input: Import Function

A patient's study can be Imported to add it into the current patient database. When this is done, the patient's scan and any work done on that scan will be stored on the PC with the other scans in the Patient List. To Import a study, click on the Import icon from the Patient List:




Then there will be a pop up box that will ask for the Input Location. Once that is provided, the study will be in the database on the current PC.

ering\PEDCAT 1022_Calibration

Output: Saving Images as JPG images

To save any one individual image as a JPG, click it to highlight and then click on the Save JPG icon, then select the location to save to.

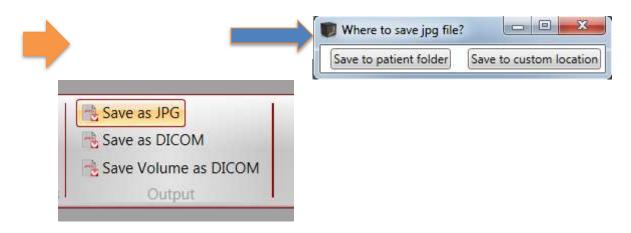

If Save to patient folder is selected, the file will save to the patient's folder and remain there. The JPG can then be exported using Media Export if desired. If Save to custom location is selected, there will be a prompt to browse to the desired location.

🗧 🕞 🗖 📔 🕨 Libra	rries 🕨 Documents 🕨	-	← Searc	h Documents
Organize 🔻 New	folder			
Desktop	Documents library			Arrange by: Folder 🔻
🖳 Recent Places	Name	Date modified	Туре	Size
詞 Libraries	Avanquest Software	10/12/2011 4:23 PM	File folder	
Documents	Bluetooth Exchange Folder	12/30/2010 11:29	File folder	
🚽 Music	🔑 eFax Messenger 4.4	11/2/2011 3:39 PM	File folder	
E Pictures	👻 🎉 Expenses	9/28/2011 11:52 AM	File folder	
File name:				
Save as type: j	og files (*.jpg)			

Output: Media Export

Burning a DISK with a free CubeVue Viewer: The software has functionality that will allow for an auto burn of a disk that contains the desired dataset(s) along with a limited-function copy of the CubeVue viewing software. The limited-function viewer does not have volume render capability. The receiving user of this disk can then open the dataset(s) in the CubeVue software for viewing. This function allows the end user to also export and burn individual images of 3D renderings, or any image of choice to the disk which can then be viewed via the CubeVue viewing software. This is useful if the receiving user does not possess one of our 3D licenses necessary for building 3D renderings. (If the receiving viewer desires to have full 3D rendering functionality, they can purchase that license through CurveBeam). Media Export will also export any CubeVue Saved Sessions associated with a dataset.

There is a Tab on the upper Menu which is called Media Export. This Tab is used specifically for creating a dataset CD with CubeVue self installer.

	Media Export
Tools and Settings	Data Series
Add CubeVue Installer	Patient Name Patient ID Date Series Description Add Series
Recipient Output To Media Burner Folder Reset Export Structure Prepare Export Export	Please select a series or multiple series from the patient list Go to Patient List Cancel
Total space required	

The first step is to click the Add Series button. This will return to the patient list for selecting a dataset(s) to burn.

• From the Patient List, highlight the desired series to be burned to the CD and right click on the series to access the new Pop-up box. Select the new item named "**Media Export**". This will automatically add the series into the Media Export list.

Patient List Rev	iew Med	ia Export				
Load Import Print List	Export DICOM Media	Reset ID	Date	Type a date 15		
Fools and Settings	•	Patient ID 🔦	Patient	Name	DOB	
	00	001	Navicular Fracture		6/4/1972	2/23/2
	00	002	First Met head non-u	nion	8/22/1959	2/23/2
	00	03	Calcaneo-navicular-c	uboid coalition	9/10/1600	2/23/2
	0004 Sesmoid fractures			9/19/1981	2/23/2	
	00	0005 Midfoot dislocation-fracture		10/6/1970	2/23/2	
	00	07	Halux Rigidus Pre-op	(5/3/1945	2/23/2
	00	0008 Lisfranc mid		dislocation-fracture 9/13/1983		2/23/2
	00	009 Post-traumatic Midfoot arthritis 4			4/24/1963	2/23/2
	10	00	Soft Tissue Wound			1/9/20
		103	First Metatarsal head	arthritic joint with cys	8	10/18/
		ype Date	Matrix 🔻	# of images	Voxel	
	R	econ 2/23/2012 2	:40 666 x 660	Media Export		200
			<u> </u>	DICOM Export		
				DICOM Send		
				Delete		


- Now click the Media Export Tab again and see the Selected Series saved in the list
- Multiple series can be added in the same method if desired.

Fools and Settings	•	Data Series			1
Add CubeVue Installer		Patient Name Sesmoid fractures	Date 2/23/2012 2:40:24 PM	Series Description Reconstructed	Add Series
Output To Media Burner Folder Reset Export Structure Prepare Export Export		1			

Also, if the user wishes to Add JPG images from this case into the Media Export Data Series List, open the series and in Review Tab, save one or multiple JPEG images to the Patient Folder. Then these will show up in the Data Series List as thumbnails. Each has a check box for selecting which to choose to be included in the Media Export. Double click on the thumbnail to enlarge for viewing if desired.

Patient List Review	Media Export	
Tools and Settings	Data Series	
Add CubeVue Installer	Patient Name Patient ID Date Series Descriptio Sesmoid fractures 0004 2/23/2012 2:40:24 PM Reconstructe rIncluded JPG Image(s)	(A)
Output To Media Burner Folder		
Reset Export Structure Prepare Export		
Export		

• Next, complete the items in the **Tools and Settings** section:

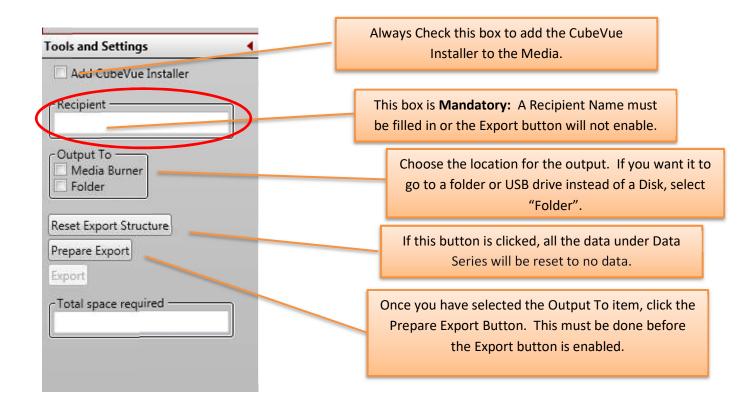


Once the Prepare Export Button is clicked, the **Total space required** field will auto fill and the **Export** button will enable.

• If selected Output is to a Media Burner (disk), **INSERT the DISK NOW** into the disk drive.

Fools and Settings	-
☑ Add CubeVue Installer	
Recipient	
Dr. Doe	
Output To Media Burner Folder	
Reset Export Structure	
Prepare Export	
Export	
Iotal space required	
393.0 MB (412,099,359.0 byte	es)


• Next, click the **EXPORT** button and the status bar will activate. When completed, a Balloon at the lower right hand corner of the screen will pop up. Click on the pop up.

(

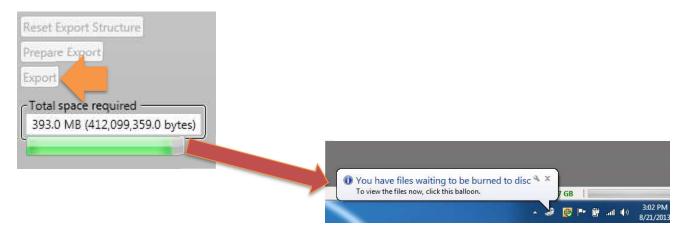


- If the Balloon disappears before you had a chance to click on it, go to START/Computer and click on the CD/DVD Burner Drive. Notice the "Files Ready to Be Written to the Disk"
- From this *Files Ready to Be Written to the Disk* Window, Click on the **Burn to Disc** button.

- This will open the Burn a Disc Window. Select With a CD/DVD Player, click Next.
- This will open the *Burn to Disk* Window. Click **Next**. This will initiate the auto burn. The CD will eject when completed.

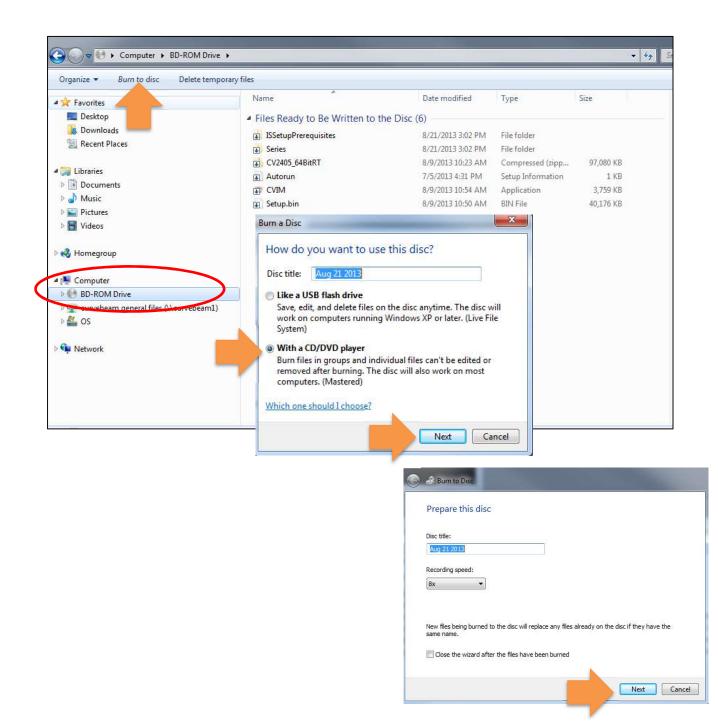

Media Export to a Folder:

- Add the desired Patient Series as described in the previous instructions.
- If you wish to perform a Media Export to a Folder or a USB Drive, select the Output To location as Folder.
 Note: a Media Export to a folder requires an Empty Folder, so it would be best to Create a New Folder to export to.
- Select Prepare Export
- Select **Export**, there will be a prompt to **Browse to** the desired folder. If there was no folder previously created, select "Make New Folder" and then name appropriately.
- Click OK.
- The Overwrite Warning message will appear if the selected folder contains ANY files. ALWAYS select an empty folder or click "Make a New Folder" to create a new folder for export, or if you click OK, then the existing files will be deleted and the Media Export files will replace them.

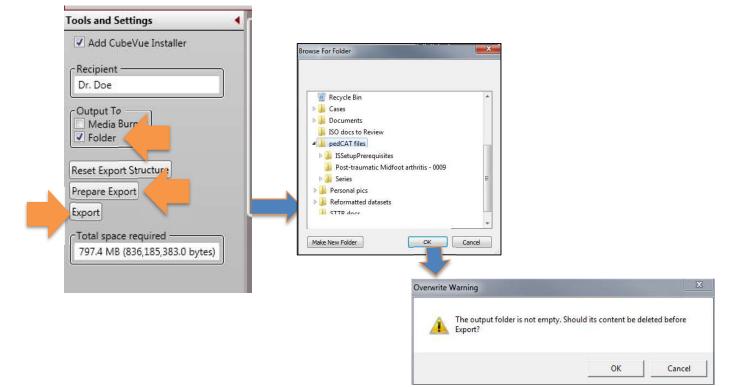


Installing a Media Export CD on a fresh computer, with CubeVue Installer

- Insert the disk into the disk drive. From AutoPlay, select **Open folder to view files on the disk.**
- Run the **CVIM.exe application** file As Administrator to launch the CubeVue Install Manager.

BD-ROM Drive - Aug 21 2013					
Always do this for software and games:					
Install or run program from your media	_	ISSetupPrerequisites	8/21/2013 3:02 PM	File folder	
Run CVIM.exe	-	😱 Series	8/21/2013 3:02 PM	File folder	
Publisher not specified		👔 CV2405_64BitRT	8/9/2013 10:23 AM	Compressed (zipp	97,080 KB
General options		J Autorun	7/5/2013 4:31 PM	Setup Information	1 KB
Open folder to view files using Windows Explorer		T CVIM	8/9/2013 10:54 AM	Application	3,759 KB
Contry Milliona Explorer		🗊 Setup.bin	8/9/2013 10:50 AM	BIN File	40,176 KB


• In the *CubeVue Install Manager*, Click **Install CubeVue & Import Data**. If CubeVue is already installed the Install CubeVue button will be disabled, so just import the data by clicking the **Import Data** button. The dataset as well as any Saved Session files and Save as JPG to patient folder files will import. Note: If there were JPEG images that were Saved to Folder on this Media, then those can now be viewed in the 3D rendering window in the Review Tab/Combined 3D/MPR Tab

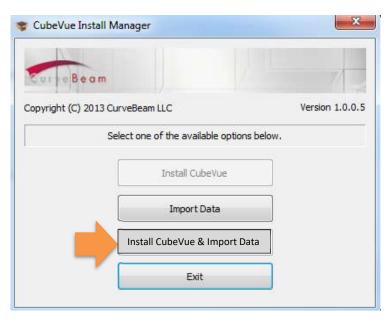

Save As DICOM

The Save As DICOM function is used to save static images in the DICOM format. The purpose of Saving static images, in DICOM format, which is simply an extension of Saving static images in JPEG format. However, the intent of this is more specific to saving images that can be sent to a PACs server or DICOM Application entity, as the JPEG images are not compatible with such systems. This would most commonly be used for saving static 3D rendering images as DICOM files

To Save an Image as DICOM, click on any desired image. The last image window that has been clicked is the Active window. Next, Click **Save as DICOM** in the Output section of the Main Menu Bar.




There will be an audio sound when clicked and the image will automatically be saved to the Patient Output folder. There will also be a message in green color at the lower left hand corner of the program that reads "DICOM IMAGE SAVED"

Multiple images can be saved in this fashion. These images are then accessible ONLY from the Patient List LOCAL Tab. These images can be loaded and viewed, Exported as DICOM, Media Exported, or also sent to a PACs server or DICOM AE. (see section on DICOM Send for instructions on sending).

mport Print List	Expor DICO Medi	M	ID	ch		Notice the # of	•
Settings	•	Patient 1000	ID Soft Tissue V	Patient Name Vound	DØB	DICOM on this	date.
to 2nd work space							
		Туре	Date	Matrix 🔷	/ # of ima	ges Voxel	FOV
		Screen	8/23/2013 9:25 AM	404 x 838	7	20120202	
		Recon	2/9/2013 3:30 PM	666 x 666	666	0.300	200
		Reformat	8/23/2013 9:22 AM	666 x 666	135	0.300	200
		Reformat	8/23/2013 9:23 AM	666 x 666	137	0.300	200
		Reformat	8/23/2013 9:23 AM	666 x 666	137	0.300	200

To View the SCREEN images in CubeVue, double click to load. Scroll the mouse wheel to advance to the next image in the Series. This series can also be loaded into the 2nd Workspace.

The functions enabled for SCREEN series are W/L, Zoom, Pan, Zoom to Fit, Reset Pan/Zoom and W/L Settings (reset). To close the SCREEN viewing window, click the "X" on the patient name Tab.

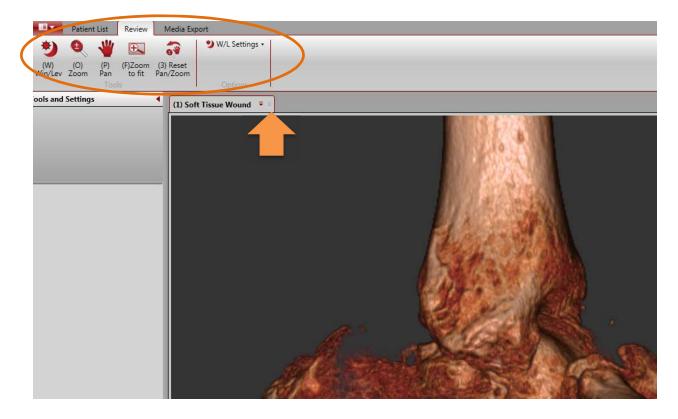

Save Volume as DICOM

The Save Volume as DICOM feature provides a method to re-save your dataset after a reorientation (volume rotation) in DICOM format. At the same time, it provides functionality to reconstruct the datasets in a format that has a larger slice thickness.

For example, the original datasets are currently reconstructed and saved at 0.3 mm voxel for MFOV scans, and 0.37 mm voxel for LFOV scans. We can utilize this new function if the dataset is desired to be sent to a PACs or DICOM server with a larger slice thickness. This may be a common need as PACs servers might not easily import the large volume of data at the smaller slice thickness.

This Save Volume as DICOM function also provides a method for reconstructing the volume in axial, coronal and sagittal planes as opposed to the original dataset, which is saved strictly as axial slices. This again may be needed for many PACs/DICOM servers.

Ultimately, from CubeVue we can now re-orient datasets and save the dataset with various slice thicknesses and outputs. We refer to these new saved datasets as "Reformats". Then we can manually send these reformatted datasets to a PACs/DICOM server as needed. (see section on DICOM Send for instructions on sending).

 To initiate the Save Volume as DICOM feature, first create the orientation that you would like to save or export, then click on the Save Volume as DICOM button from the Main Menu Output section from the Review Tab/Combined 3D MPR Tab. This will open the DICOM Volume Creation Window.

Save as JPG		DICOM Volume Creation
Output	Select vew direction from slab window frame color	Choose output geometry Slice Thickness: 0,3 mm Slice Spacing: 0 mm
	Progress : Select view direction(s)	Start Close

From this window, first select the desired **View Direction:** In most cases, all of the view directions would be selected. *Red = axial, Green = sagittal, Blue = coronal.* However, there may be an event where only Red (axial) is necessary.

	■ DICOM Volume Creation
Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction from slab window frame color Image: Select vew direction f	Choose output geometry Slice Thickness: 0.3 mm Slice Spacing: 0 mm
Series Description : CT LE LEFT WITHOUT CONTRAST Series Description : CT LE LEFT WITHOUT CONTRAST Series Description : CT LE LEFT WITHOUT CONTRAST Progress :	Notice that once the view direction is selected, the series description for each is displayed. These descriptions can be edited, click inside the field for access to the text.
	Start Close

• Next, select the desired **Output Geometry**, then click **Start**. The default for slice thickness will display as either 0.3 mm for a MFOV scan or 0.37 for a LFOV scan. The options are to either click on the drop down menu and select 5x, 10x or 15x. Or you can drag the scroll bar for additional options in the current slice thickness with increments.


5X is recommended in most cases and should be suitable for most needs. For a MFOV, 0.3 mm voxel scan: 5x = 1.5mm slice thickness For a LFOV, 0.37 mm voxel scan: 5x = 1.85 mm slice thickness

		DICOM Volume Creatio."
	from slab window frame color Red reen Blue	Choose output geometry Slice Thickness: 1.5 mm Slice Spacing: 0 mm 5x v 5x 1.5 mm 1.5 mm 5x v 1.5 mm
Series Description :	CT LE LEFT WITHOUT CONTRAST	15x
Series Description :	CT LE LEFT WITHOUT CONTRAST	
Series Description :	CT LE LEFT WITHOUT CONTRAST	
-		
Progress :		

• Once the Status reads Completed, click Close. The new Reformatted Datasets will reside under the Patient ID, Series Type in the Patient List LOCAL Tab only. The Series Type will be called Reformat.

Patient List Review	Media Export							
Import Print Hide Ex List List DIG	port COM edia	Name sof ID Searc	Date Type a date	•				
Settings 🔹	Patient	ID	Patient Name	DOB	Study	Date 🔻		Description
	1000	Soft Tissue V	Vound		1/9/2013 3:22 F	M	Wound_unexplained pain	
nto 2nd work space								
	Туре	Date	Matrix 🔶	# of images	Voxel	FOV	DAP Filter Protocol Description	
	Screen	8/23/2013 9:25 AM	404 x 838	7			ULTRASHARP	CT LE LEFT WITHOUT CONTRAST
	Recon	2/9/2013 3:30 PM	666 x 666	666	0.300	200	ULTRASHARP	CT LE LEFT WITHOUT CONTRAST
	Reformat	8/23/2013 9:22 AM	666 x 666	135	0.300	200	ULTRASHARP	CT LE LEFT WITHOUT CONTRAST
	Reformat	8/23/2013 9:23 AM	666 x 666	137	0.300	200	ULTRASHARP	CT LE LEFT WITHOUT CONTRAST
-/	Reformat	8/23/2013 9:23 AM	666 x 666	137	0.300	200	ULTRASHARP	CT LE LEFT WITHOUT CONTRAST
	Local	lemote	-					

If you desire to delete any of these datasets, click on to highlight, right click for the pop up menu, select **Delete** from the menu. Select multiples by holding down the CTRL button then click each desired dataset.



Note: Reformat datasets **Will NOT open** in CubeVue software. These datasets are no longer isotropic and not intended to be viewed in CubeVue. The original Reconstructed (RECON) datasets should be used to view in CubeVue.

DICOM Send

Any of the datasets that reside in the Patient List LOCAL Tab can be sent to a PACs/DICOM server via the DICOM Send functionality. In most cases, the Series Types that will be desired to send via this method would be SCREEN and REFORMAT datasets.

From the Patient List LOCAL Tab, **highlight any or all of the desired Series to send**. Highlight multiples using the traditional method of CTRL click, or highlight all using the traditional method with SHIFT, click on the first and SHIFT click on the last.

 Right click on the highlighted dataset(s) to access the Pop Up menu and select **DICOM** Send.

Patient	t ID	Patient Name				
1000	Soft Tissue W	/ound				
Туре	Date	Matrix 🔦	# of in			
Screen	8/23/2013 9:25 AM 404 x 838		7			
Recon	2/9/2013 3:30 PM	666 x 666	666			
Reformat	8/23/2013 9:22 AM	135				
Reformat	8/23/2013 9:23 AM	666 x 666	137			
Reformat	8/23/2013 9:23 AM	Media Export	137			
		DICOM Export				
		DICOM Send				
		Delete				

• This will open the *DICOM Sender* Window. In this window, one or multiple **Destinations** for the data send can be configured. Configure a Destination with the appropriate data and click the **Update** button to Save. To add another Destination, click on **New** and edit the Destination items, click Update to Save. Once there are Destination(s) configured, they will remain in the list unless deleted.

				ALC: NOT THE OWNER OF THE OWNER OWNER OF THE OWNER OWNE		and the second	
Destination			P	lew: to	configure	one or m	ore additional Des
Name :	PACs1	PACs1					
Host :	10.1.10.1189	PACs2	/ L	Jpdate:	to Save a	New Des	tination
Port :	11112		/ C	Delete:	to delete a	highlight	ted Destination.
Local AE :	CUBEVUE		/ -				
Remote AE:	PEDCAT	New	Up	date	Delete		
Progress Status : C	lick 'Start' to begi	0,					

- Click **Start** to begin the Send. The Send time will depend on how many datasets and destinations are selected, the number of reformats created, and the speed of the PACS network.
- When the Send is completed, the Status will read "Completed".

APPENDIX I: PedCAT Installation Instructions

WARNING Use of controls or adjustments or performance of procedures other than those specified herein may result in hazardous X-ray radiation or laser light exposure.

The PedCAT Machine will be skidded or crated and shrink wrapped for shipment. The crate should remain upright as instructed on the crate. Please inspect all components and advise CurveBeam of any damage to the crate or items within the crate upon delivery.

The skid will contain:

- 1. The machine itself.
- 2. External Server
- 3. 2 Handle Bars

4. 4 boxes containing a thin client terminal, PC, medical grade monitor, control box, cables, phantoms, carbon fiber platform plate, accessories.



Machine shipping mount/bolts.

1. De-skidding the machine:

The machine first needs to be unbolted from the skid. The shipping mount/bolts are in the front of the machine. Then, the rear cover should be removed before attempting to slide the machine off the crate or else it will be damaged. Once the rear cover is removed, the back of the unit should be slid to the edge of the skid so the 2 rear wheels are hanging off the edge, then lift the unit upright. It will slide down the edge of the skid on to the wheels.

The Unit should be lift gated to ground (onto a dolly if necessary) or by the wheels and rolled into the facility in the upright position:



2. Remove Shipping clamps, ties & screws:

Once the machine is in the area of placement, perform the following:

This Clamp should first be removed:




The underside of the machine has 2 securing cable ties on each side under each door motor which lock down the doors for shipping. And the top of the machine has securing cable ties to help keep the gantry secure. These all must be snipped and carefully removed.



Then the 4 Gantry Clamp Shipping screws can now be removed. These secure the gantry during shipment. They are at the base of the gantry.




3. The back Power Panel has been placed in a "Shipping" position to secure during shipping. This needs to be adjusted to its operational position. Remove the top 2 screws. The remaining 2 mounting screws are stored below the panel.



Shipping position of back Power Panel. Remove these 2 top screws

The 2 remaining mounting screws are stored here below the panel.

Once the 2 screws are removed, pull the Power Panel out to its operational position and secure into place with the 4 mounting screws.

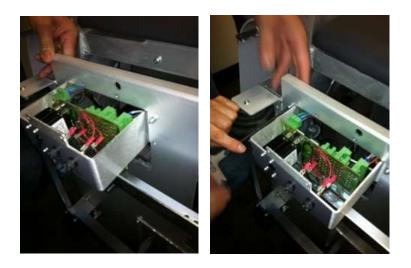


4. At the location of placement, set the machine down on its base.



- If being placed with the rear to the wall, be sure to leave some room in the back in order to plug in all cables and for securing the rear cover before placing the machine into its final spot.
- There are a total of 4 adjustment "feet" to the machine, one at each corner. There is also a center foot that has no adjustment. The machine should sit on the center foot and lean back onto the 2 back feet. The 2 front feet should not yet be touching the floor at this time. They will be adjusted once the machine leveling is complete.



- 5. Attach all cables and cords to the back of the machine:
 - a. Machine power cord
 - b. Operator's control box
 - c. Door interlock connector
 - d. X-ray warning connector
 - e. 2 CAT 6 ethernet cables that feed to the server. One will be labeled Red for the Red cable and one will be labeled Green for the Green cable.

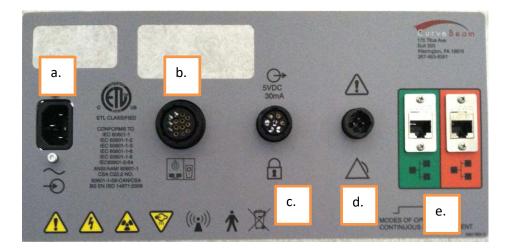

Control Box (b.)



6. Check All connections on boards, circuits etc in the system. Ensure that all are seated.

7. Mount the Varian Receptor Panel:



- a. There are 3 cables to be attached.
- CAT6 cable (cable tie this cable to the black clip to maintain security).
- Power cable
- Ground cable
- b. The Ground nut should be removed from its location, then attach the ground cable and re-attach the Ground nut.



- c. Attach the Panel with 4 Plate screws.
 - The Load position of the panel is in the Gantry "B" position, which is centered.
 - Begin by securing the first 2 screws (vertically) and then manually move the panel to the Gantry Home position, which is rotated to the right, with your hands and secure the other 2 screws (vertically).

- d. Check for Level of the Panel when mounting.
- e. Check for Pivot of the Panel when mounting. The pivot may need to be fine tuned during the panel alignment procedure that will be completed at completion of installation. If the pivot requires adjustment, use the pivot adjustment screws on the panel mount.



8. <u>Mount the X-Ray tube head:</u> There is only one twist lock connector and 4 screws for mounting.





9. Mount the Patient Handle Bars:

- There are 2 bars, each is mounted with 2 Screws.
- Each bar has a Ground cable that needs to be attached to the ground screw.



10. Level the Patient Platform:

- Before leveling the platform, be sure to verify that the platform/gantry is stabilized. This can be checked by pulling & pushing the gantry towards & away from the center of rotation, there should be no play. If there is play, you must tighten the screw underneath. The patient platform must be removed to get to this screw.
- The machine should be leveled for left/right and front/back. Place a level on the patient platform area without the plastic platform plate in place.
- Adjust each of the 2 back feet up and/or down to achieve level.
- Once level is achieved, adjust the 2 front feet down to the ground for support.

11. Check Laser Light Alignment:

WARNING Use of controls or adjustments or performance of procedures other than those specified herein may result in hazardous laser light exposure.

There are 3 laser lights, one vertical in center of rotation, 2 horizontal at 10cm height and 20 cm height.

Vertical laser light: this should be aligned to the platform center screw as depicted in the below image. If not, adjust it via the adjustment screw on the vertical laser light mechanism to achieve proper location, circled in the below image.



Horizontal Laser Lights: The lower light should be 10 cm above the platform. The upper laser light should be 20 cm above the platform. If not, adjust each adjustment screw on the horizontal laser light mechanisms to achieve proper location.



12. Server Setup:

The External server consists of 4 Virtual Machines, on the right hand side. It is contained in a case that also has a UPS unit, on the left hand side. The first step will be to plug in the UPS Battery Plug, located beneath the UPS cover.



Remove the left cover from the bottom clip. Connect the battery plug. Turn the UPS ON with the button below the plug and verify that it is powered. Replace the cover.



Plug in all cords in the back of the case:

- 2 CAT6 Ethernet cables (Red & Green)
- 2 cables from Server to each of the 2 Thin Client Terminals.
- 2 power plugs from the server to the UPS unit.
- 1 Power cord.
- HUB (switch for the thin client terminals)



Turn ON the server and verify that all VM's are powered ON. You must remove the right hand side cover to access the ON button to the server.

Connect the ACQ Thin Client Terminal to the HUB, and connect the HUB cable to the server. Plug in the Thin Client Terminal box, Monitor and mouse. Turn the Thin Client Terminal box ON.



Connect the Viewing Station/MD Thin Client Terminal to the server. Plug in the Thin Client Terminal box, Monitor and mouse. Turn the Thin Client Terminal box ON.



13. Turn the Power to the machine ON from the Main Circuit Breaker at the back of the machine. This is the only ON button for the machine. ON position = I, OFF position = 0.



- 14. Once all connections are secure and the machine is Powered ON, launch the ACQ Connection from the icon on the Main Connection Desktop of the ACQ Thin Client Terminal.
- 15. Once connected to the ACQ Desktop, launch the PedCAT ACQ "CB Scanning Device" software from the icon. Verify StartUp/Initialization has completed. Each of the on-screen lights should light up. During the startup/initialization observe the machine for any vibration, unexpected performance or deterioration of performance.



The StartUp sequence is designed to run diagnostics to ensure that all components of the systems are functioning as expected. There are checks for communication to the data storage (DICOM VM), communication with the firmware, and operation and homing of all motors which include the gantry motor, panel motor, beam limiter motor and both door motors. If there is a failure in any of these, the software will not advance to the scan Acquisition section.

- 16. If all initializes properly, attach the rear cover with the 4 button screws and push the machine to its final position. If there is a StartUp issue, please re-check all connections, reboot the machine and attempt again. If an issue continues, please contact CurveBeam Technical Support.
- 17. Follow ALL the Alignment, Calibration QA procedures outlined in **Chapter 4** of this manual. INSTALLATION is NOT COMPLETE until all these procedures are successfully completed.

APPENDIX II: Troubleshooting

Error Messages:

System failures that may result in a scan failure will be accompanied by Error Messages in the software. The user should follow the instructions to resolve the error, however if the Warning message persists, the user should contact CurveBeam technical support at 267-483-8081. If the system fails to operate in any other way or if your problem is not listed, please contact CurveBeam technical support at 267-483-8081.

Firmware Monitoring Warning: Upon startup of the "CB Scanning Device" Acquisition software, the system checks that the embedded controller firmware software version is the correct version to operate with unit. If an unsupported version number firmware software resides on the embedded controller then the following error message will display and the Acquisition software will terminate. In the event of this error message, please contact CurveBeam technical support.


8
ted by this
r

Temperature Monitoring Warnings: The system is designed to send a Warning message to the user if the internal temperature of the machine is below 35° C or above 45° C. This Warning would display in the "CB Scanning Device" Acquisition software at Startup and just before a scan is captured. If the temperature is below the 35° C limit then the resulting image quality may not be optimal, however the system will permit scanning (for either upper or lower temperature conditions).

The Warning message reads:



Startup: Note that there is an Internal Temperature gage in the Startup Screen. If in the Startup Screen and the temperature monitor has detected temperature out of range, the warning message will display during the Startup sequence.

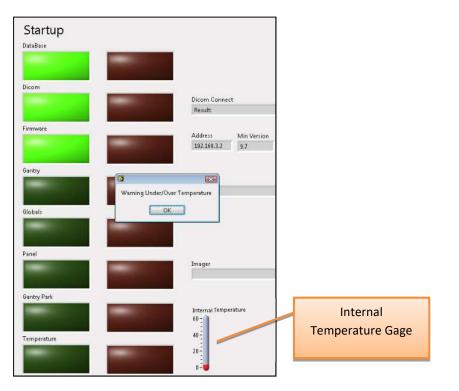

Scan: If in the Procedure Tab and the temperature monitor has detected temperature out of range, the warning message will display once the OK button is clicked.

Patient Name	Procedure / Protocol	
b reaker	/(Partial single foot, Normal Filter: 20D x 20H, 0.3 vox)	1
Procedure Stage Doors Closing		2-
Notes	S Warning Under/Over Terr	eperature
% Complete	OK	
ok		


Temperature Monitoring Failures: The system is designed to send a Failure message to the user if the internal temperature of the machine is 20° C or lower OR 60° C or higher. This Failure message would display in the "CB Scanning Device" Acquisition software at Startup and just before a scan is captured. If this condition occurs the error message will force the acquisition program to terminate and disallow any scanning.

In the event of such Failure message, the user should re-start the system via the Circuit Breaker ON/OFF switch and then re-launch the "CB Scanning Device" Acquisition software. If the message still displays, the user should contact CurveBeam technical support.

The Failure Message reads:



Startup: Note that there is an Internal Temperature gage in the Startup Screen. If in the Startup Screen and the temperature monitor has detected temperature out of range, the failure message will display during the Startup sequence.

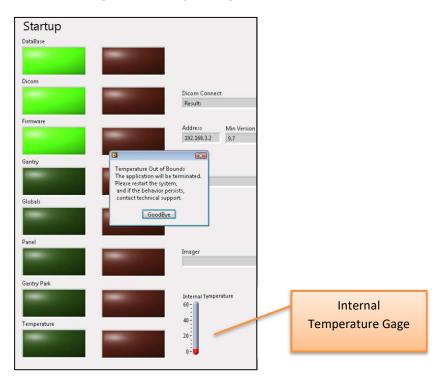

Scan: If in the Procedure Tab and the temperature monitor has detected temperature out of range, the failure message will display once the OK button is clicked.

Patient Name	Procedure / Protocol	
b reaker	/(Partial single foot, Normal Filter: 20D x 20H, 0.3 vox)	1
Procedure Stage Doors Closing		-9000
Notes	Temperature Out of The septication will be	Rounds
	Please restart the syst and if the behavior p contact technical sup	tem, iersists, pp.ort.
% Complete	GoodBy	
Start		
QK.		-0

Beam Collimator Mechanism Failure: The beam collimator is a motorized mechanism which select position dependent on the scan procedure selected. An error message will display if there are any issues with the motor, such as a stall or jam, or switches that control the movement of the beam collimator mechanism. This message can display at Startup screen or in the Procedure Tab as the system sets up for the scan.

18	X
a reference positio	
The application wil Please restart the sv	
and if the behavio	
contact technical :	support.
C	GoodBye

Panel Position Mechanism Failure: The Panel Position Mechanism is a motorized mechanism which selects its position dependent on the scan procedure selected. An error message will display if there are any issues with the motor, such as a stall or jam, or switches that control the movement of the Panel Position mechanism. This message can display at Startup screen or in the Procedure Tab as the system sets up for the scan.

•••
Panel Transport Motortimed out while seeking a reference position
The application will be terminated.
Please restart the system,
and if the behavior persists,
contact technical support.
GoodBye

Gantry Rotation Position Mechanism Failure: The Gantry Rotation Mechanism is a motorized mechanism as well. An error message will display if there are any issues with the motor, such as a stall or jam that would result in the Gantry not finding its proper positioning. This message can display at Startup screen or in the Procedure Tab as the system sets up for the scan.

C _B	X
Gantry Rotation The application will be terminat Please restart the system, and if the behavior persists, contact technical support.	ed.
GoodBye	

An error in Gantry Rotation *during a scan* would result in a communication error of the receptor panel to the server, so if this even occurs, the following Panel Readout error message would display:

C
Panel Readout The application will be terminated. Please restart the system, and if the behavior persists, contact technical support.
GoodBye

Gate Drive Mechanism Failure: The Gate Drive Mechanism is a motorized mechanism which opens and closes each door at the appropriate times. An error message will display if there are any issues with the motors, such as a stall or jam, or switches that control the movement of the Gate mechanism. This message can display at Startup screen or in the Procedure Tab as the system sets up for the scan.

3	×
Gate Drive Motortimed a reference position	out while seeking
The application will be t	erminated.
Please restart the system	۱.
and if the behavior pers	ists,
contact technical suppo	ort.
GoodBy	e i
And the second s	

Panel Read Out Error Message: If any communication failure occurs before or during a scan between the receptor panel and the server, then a Panel Readout Error will display on Screen. Communication errors could occur if the cable is not plugged in or seated correctly or has suffered some damage, or if the panel does not properly produce frames. The "CB Scanning Device" Acquisition software will terminate. Check cables and Restart the system.

ü n	
Panel Readout The application will be terminated. Please restart the system, and if the behavior persists, contact technical support.	
GoodBye	

Communication Error between the Firmware and the Server: If there is any loss of communication between the embedded controller firmware, the following error message will display on screen. Loss of communication can be caused by a damaged, unplugged or loose embedded controller cable, or when the Emergency Stop button has been pressed. The "CB Scanning Device" Acquisition software will terminate. Check cables and E-stop and restart the system.

MicroController Sequence Error The application will be terminated. Please restart the system, and if the behavior persists, contact technical support.
GoodBye


Exposure Timeout Error Message: In the event of a system fault that may result in the X-ray exposure not terminating at its appropriate time, there is a backup timer to terminate the exposure. If this occurs, the below error message will display on screen. Click OK and restart the system. If the error occurs again, contact CurveBeam Technical Support.

ament Timeout During Scan	
ERROR: Filament Timeout During Scan	

Scan Button Released Error Message: If the operator releases the scan button BEFORE completion of an exposure, the X-ray will turn off and the below error message will display notifying the user of the error.

If this occurs, the operator should review the reconstructed data to determine if the data capture was sufficient for diagnosis. If not, a new scan may be necessary.

ERROR: Scan Button Released During Scan	
ок	

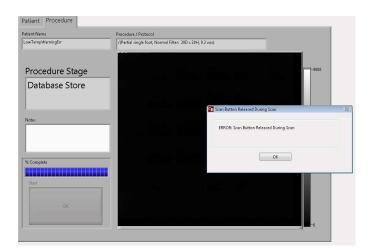


Calibration Checks and Services Warnings: The system calls for monthly Panel Calibrations and checks of certain control functions as outlined in this manual. A monthly Warning message will appear that will indicate that it is time for these checks.

The Warning message reads:


Eq.	
	System Out Of Calibration Calibrate Immediately
	ОК

Startup: When the monthly calibration and checks are due, the message will display during the Startup sequence. The user should click OK and then should contact

CurveBeam technical support who will assist in the calibration and checks via remote access. This message will repeat at Startup until the procedures are completed. Once the procedures are completed the warning message will be reset by CurveBeam technical support.

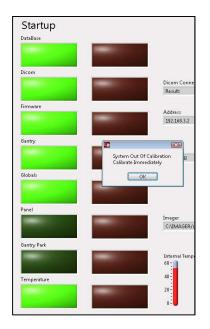

Scan: When the monthly calibration and checks are due, the message will display in the Procedure Tab when the OK button is clicked. When the message displays, the user should click OK and then should contact CurveBeam technical support who will assist in the calibration and checks via remote access. This message will repeat at Scan time until the procedures are completed. Once the procedures are completed the warning message will be reset by CurveBeam technical support.

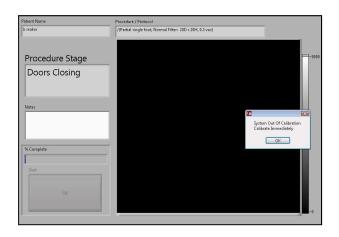

QA Service and Maintenance Warnings: The system calls for annual QA procedures and system maintenance as outlined in this manual. An annual Warning message will appear that will indicate that it is time for these services.

The Warning message reads:


ű:		X
	System Maintenance	
	Needed Immediately	
	ОК	
-		

Startup: When the annual service is due, the message will display during the Startup sequence. The user should click OK and then should contact CurveBeam technical support who will schedule the service and maintenance. This message will repeat at Startup until the procedures are completed. Once the procedures are completed the warning message will be reset by CurveBeam technical support.

Startup	
DataBase	
	-
Dicom	
Contract of the second s	Dicom Connect
	Result
Firmware	
and the second se	Address Mir 192,168,3,2 9,7
	192,100.3.2 3.7
Gantry	
and the second se	System Maintenance
	System Maintenance Needed Immediately
Globals	OK
Panel	
	Imager
	C:\IMAGERs\C306-0
Gantry Park	
	Internal Temperature
Temperature	40-
	20-
	0-

Scan: When the annual service is due, the message will display in the Procedure Tab when the OK button is clicked. When the message displays, the user should click OK and then should contact CurveBeam technical support who will schedule the service and

maintenance. This message will repeat at Scan time until the procedures are completed. Once the procedures are completed the warning message will be reset by CurveBeam technical support.

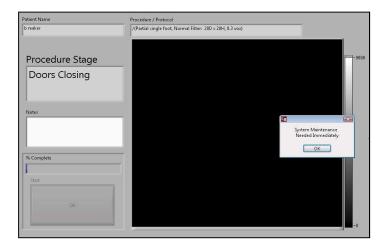

APPENDIX III: Scan Protocol Technical Details

pedCAT Study Type:	Foot and Ankle Cone Beam CT
Scan Positions/Orientations:	Weight Bearing (standing), Seated (partial or non weight bearing)
CT Scanner make and model:	CurveBeam pedCAT
Maximum # of Slices per acquisition:	N/A: System is Volume Cone Beam CT

pedCAT has 5 Scan Protocol options:

Acquisition series (include all) (i.e., axial, helical)	Medium Field 100 kVp (small patient)	Medium Field 120 kVp	Large Field 100 kVp (small patient)	Large Field 120 kVp	Medium Field Sharp, 120 kVp
kVp/mA and rotation time or kVp/mAs	kVp = 100 mA = 5 mAs = 22.62 Rotation time = 16 seconds	kVp = 120 mA = 5 mAs = 22.62 Rotation time = 16 seconds	kVp = 100 mA = 5 mAs = 45.24 Rotation time = 32 seconds	kVp = 120 mA = 5 mAs = 45.24 Rotation time = 32 seconds	kVp = 120 mA = 5 mAs = 22.62 Rotation time = 16 seconds
CTDI (vol) required (if on system)	0.47 mGy	0.89 mGy	0.63 mGy	1.10 mGy	0.89 mGy
Dose length product (DLP) required if on system	-	-	-	-	-
Total dose per acquisition and/or total dose per study if available in units given	Dose Area Product = 5.05 dGy*cm²	Dose Area Product = 8.30 dGy*cm ²	Dose Area Product = 9.30 dGy*cm ²	Dose Area Product = 15.45 dGy*cm ²	Dose Area Product = 8.30 dGy*cm ²
Tube current modulation or dose reduction technique (is used)	12 millisecond pulsed. 377 pulses/scan	12 millisecond pulsed. 377 pulses/scan	12 millisecond pulsed. 754 pulses/scan	12 millisecond pulsed. 754 pulses/scan	12 millisecond pulsed. 377 pulses/scan

		-	-	-	
Anatomical Scan range (i.e., dome of liver thru pubic symphysis)	L or R Ankle and midfoot <i>or</i> L or R midfoot & forefoot	L or R Ankle and midfoot <i>or</i> L or R midfoot & forefoot	L or R Ankle and entire foot <i>or</i> bilateral feet and ankles	L or R Ankle and entire foot <i>or</i> bilateral feet and ankles	L or R Ankle and midfoot <i>or</i> L or R midfoot & forefoot
Increment (space between slices)	0 mm	0 mm	0 mm	0 mm	0 mm
Detector collimation (mm)	Fixed 7-8% of detector, factory calibrated	Fixed 7-8% of detector, factory calibrated	Fixed 7-8% of detector, factory calibrated	Fixed 7-8% of detector, factory calibrated	Fixed 7-8% of detector, factory calibrated
Slice thickness (mm)	0.5mm +/-0.5mm	0.5mm +/-0.5mm	0.5mm +/-0.5mm	0.5mm +/-0.5mm	0.5mm +/-0.5mm
Slice spacing (mm)	0.30mm	0.30mm	0.37mm	0.37mm	0.30mm
Pitch or table feed	0	0	0	0	0
Scan FOV (cm)	20 cm diameter x 20 cm height	20 cm diameter x 20 cm height	35 cm diameter x 20 cm height	35 cm diameter x 20 cm height	20 cm diameter x 20 cm height
Kernel/filter	-	-	-	-	Sharp
Reformat technique (i.e., 3D, plane/views)	Automatic (coronal/sagittal volumes optional)	Automatic (coronal/sagittal volumes optional)	Automatic (coronal/sagittal volumes optional)	Automatic (coronal/sagittal volumes optional)	Automatic (coronal/sagittal volumes optional)
Contrast type/rate (if applicable)	Not Used	Not Used	Not Used	Not Used	Not Used
Time from contrast injection to image acquisition, if applicable (sec)	Not Used	Not Used	Not Used	Not Used	Not Used

APPENDIX IV: Advanced Calibrations

The calibrations here are accessed via CB-ToolShed with a password and are considered advanced calibrations, not for the user to perform. These Calibration Procedures should be performed only by factory trained technicians.

To complete all of the calibrations, allow at least 2 hours. Perform them all in the order presented.

The tools required for Calibration: Centering Tool Geometric Phantom QA Phantom (Line Pair Phantom) Water Phantom

Ensure that all safety precautions are taken for the location in which these procedures are being performed. If the office is equipped with the Door Interlock Option, ensure that the appropriate measures are taken to be able to perform a scan and fire the x-ray. If needed, there is always the option to release the Scan button or to use the E-Stop to stop the x-ray in the middle of a calibration. If the E-Stop is depressed, it will cause the power switch on the back of the scanner to shut off. Reset the E-Stop by rotating it, then restart the scanner by flipping on the power switch at the back of the scanner. Then restart the calibration at the beginning of the calibration that was interrupted. If the scan button is released prematurely during a calibration, rerun the current calibration.

Open CB-ToolShed and enter the required password to access the advanced calibrations.

Geometric Calibration

Locate the Geometric Phantom and the Patient Platform. The Platform should be in place in the scanner. Then Patient Platform has positioning circles drawn on it to allow for aid in proper positioning of the Geometric Phantom. Place the Geometric Phantom in the center of the Platform, using the positioning circles as guides to find the approximation of center. Once placed, it will look similar to the following image:



The Geometric Calibration will need to be run on both a MFOV and a LFOV scan, but only one of each. For the purposes of viewing the BB's better, the 120 kVp scans should be used. This procedure will be run first using the Large Field (120 kVp) scan and then again using the Medium Field (120 kVp) scan.

Click on the tab labeled Geometric Analysis and File Creation to get started with the Geometric Calibration. The Geometric Calibration tab will appear as follows:

B Side	Center	A Side
A b 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0 0		
J	Select Protocol	
A/B/Center Distance Measurement		View Cal Files Firmware Reconstruction Log DataBase Single Shot Motor, LED, Xray Control
General System Information In	Regulity Analysis Panel Gain Calibration	Normalization File Creation for Reconstruction engine Geometric Analysis and File Creation Find Center of rotation
Protocols CeoCa	al Phantom Must Be Centered	
Mame		orm Geo (a) 90.4-
Large Field (120 kVp)	12/17/2014 3:26 12/15/2014 4:47 12/15/2014 3:15 P 12	or no sine wave
Medium Field (120 kVp)	2/17/2014 3:38 12/15/2014 4:23 12/15/2014 3:15 P 12	
Medium Field, Sharp Filter(120 kVp)	2/17/2014 3:43 12/15/2014 4:28 12/15/2014 3:15 P 12	2/15/2014 3:23 P 11/20/2014 10:35 90 - riance riance
Small Patient: Large Field (100 kVp)	12/19/2014 10:3€ 12/15/2014 4:34 12/15/2014 3:15 P 12	
Small Patient: Medium Field (100 kV)	12/15/2014 4:12 12/15/2014 4:38 12/15/2014 3:15 P 12	80.7-
		0 100 200 300 400 0.0000 0.0000
		Frame In range Capture Geocal
		Instructions will Ende
 		17:37 OK
		appear here
	1962-01-1- 049440-02-02-1 16-46-14-14	
Room Door Ready	Xray Service Fault	Complete Busy
		EXIT

Highlight first the Large Field (120 kVp) scan then click on the Capture Geocal OK button. Instructions will be visible and will instruct the user when to fire the x-ray. The x-ray will need to be fired during this calibration. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

The x-ray will need to be fired twice for this Large Field scan. When prompted, Press and Hold the Scan button to fire the x-ray for the second pass for the Large Field.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

While the x-ray is firing the screen will go light gray and images will appear in the boxes at the top, similar to below:

760.765 0.36X Unsigned 16-bit image 43600 0.0	Q ₩0 %\\ Q A A D % A D % A D % A D % A A D % A A D % A A D % A A A A	€ + - - - - - - - - - -	7768 0.36X Unsigned 16-bit image 43600 (0,0)
Large Field (120 kVp) 12/17/2014 3:25 Medium Field (120 kVp) 12/17/2014 3:33 Medium Field, Sharp Filter(120 kVp) 12/17/2014 3:43 Small Patient: Large Field (100 kVp) 12/17/2014 1:03		es 00.4 (x0/2014/277) 00.2- 01/20/2014/271 00.2- 01/20/2014/271 00.2- 01/20/2014/271 00.2- 01/20/2014/271 00.2- 01/20/2014/271 00.2- 01/20/2014/271 00.2- 01/20/2014/271 00.2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 01/20/2014/271 00/2- 02/2-	e Single Shot is and File Creation Left Side Find Center of rotation The average should be average avera

Another program will also open to assess the BB's, but will not require user input, the screen will look similar to the following:

K IsoCal for CST						1			من ریکی رولیک
VAR AN medical systems	Load Data Set	System Setup	Auto Position	Unlock Gates		Þ	Help About		
				•					
			•	•	•			768 0.36X Unsigned 16-	bit image 43690 (0,0)
			•					Single Shot and File Creation	
				•				Left Side Right Side Average Mean / Std D \$0 89,9508 0.005	
			·		•			90.0016 0.056 89.9762 0.06 In range	
_									ОК
									EXIT

Next a pop up box will appear as shown below:



Click OK. The same pop up box will appear a second time, again, click OK.

Once the calibration is done for the current protocol, check the status of the lights. The only lights lit up should be green, if they are not green, contact Technical Support. Additionally, the current date and time should be entered in the "Geo" column on the row with the scan protocol just completed, similar to the below image:

< 			that da	e		it image 43690		03	(768x768 (-bit image 43690 (0,0)
A/B/Center Distance Measurement	Advanced Q	undat	ed here		iles	Firmware	Reconstruction		taBase	Single Shot	
General System Information Ima	age Quality Ana	upuan	eu nere	2	ation File	Creation for Red	construction engine	Geometric A	Analysis an	d File Creation	Ensure only
Protocols GeoCa	Phantom w	изт ве сеп	terea						_		green lights
Name	LP	Water	Gain Cal	Norm	Geo	19	90.2-			eft Side	greeningnis
Large Field (120 kVp)	12/17/2014 3:26	12/15/2014 4:47	12/15/2014 3:15 P	12/15/2014 3	5 P 12/1	9/2014 11:39	90.1-		R	light Side 📈	here
Medium Field (120 kVp)	12/17/2014 3:38	12/15/2014 4:23	12/15/2014 3:15 P	12/15/2014	P 12/1	9/2014 11:28	90 -	hallon de	A	verage 📈	nere
Medium Field, Sharp Filter(120 kVp)	12/17/2014 3:43	12/15/2014 4:28	12/15/2014 3:15 P	12/15/2014	23 P 12/1	9/2014 11:28	89.9-				JEV / Vanance
Small Patient: Large Field (100 kVp)	12/19/2014 10:3	6 12/15/2014 4:34	12/15/2014 3:15 P	12/15/2014 3	26 P 12/1	9/2014 11:39	89.8 -		\$0 \$0	0 89.9508 0.08	154 0.0073
Small Patient: Medium Field (100 kVp)	12/15/2014 4:12	12/15/2014 4:38	12/15/2014 3:15 P	12/15/2014 3:	2° P 12/1	9/2014 11:28	89.7 -		鈔	90.0016 0.05	65 0.0032
							0 100	200 300	400	89.9.52 0.06	76 0.0046
2								Frame		n range	
							Last Maintenance	Date			Capture Geocal
					_		2014-12-19 11:39				
4			1	1		+	2014-12-19 11:39	15			OK
Room Door Ready	Xray	Service	Fault	Co	mplete	Busy					
						Dusy			الله الم يعا في ا		EXIT
	and the second se										

Once the Large Field (120 kVp) has completed and has green passing lights, **repeat the Geometric Calibration procedure for the Medium Field (120 kVp) protocol**.

Find Center of Rotation

Remove all objects from the Field of View in the scanner.

Remove the Patient Platform from the scanner.



Place the Centering Tool **Constant** into the center of the metal disc from where the patient platform was removed. There are 2 holes on the metal disc that will fit the two metal prongs at the bottom of the centering tool. The Centering Tool will fit in one of two ways, either way is acceptable for this procedure.

Holes in metal disc in the patient platform area (with patient platform removed):



Center tool properly placed:



	3 Side		Center		A Side	
Q ₩ 0+\\□\\+@ %	٠			,		, ,
<u>1</u>		Select F			<u> </u>	
	A/B/Center Distance Measurement	Advan			Log DataBase Single Shot	Motor, LED, Xray Control
	General System Information Imag					
	ocherar system monnation and	ge Quality Analysis Panel	Gain Calibration	Normalization File Creation for Reconstruction engine	Geometric Analysis and File Creation	Find Center of rotation
- 1	/	ge Quality Analysis Partel	Gain Calibration	Normalization File Creation for Reconstruction engine	Geometric Analysis and File Creation	Find Center of rotation
	Protocols					Find Center of rotation
	Protocols	LP Water 12/17/2014 3:26 12/15/2014 4:47	Gain Cal Norn	n Geo Place Centerir	ng Tor	L :ol
	Protocols	LP Water	Gain Cal Norm	n Geo Place Centerir 5/2014 3:35 P 12/19/2014 11:39		:ol gain and offset
	Protocols Nam Large Field (120 kVp) Medium Field (120 kVp) Medium Field, Sharp Filter(120 kVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 2/17/2014 3:38 12/15/2014 4:28 2/17/2014 3:43 12/15/2014 4:28	Gain Cal Norn 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n Geo Place Centerir 5/2014 3:35 P 12/19/2014 11:38 5/2014 3:24 P 12/19/2014 11:28 5/2014 3:29 12/19/2014 11:28	Click to start	col gain and offset lone before this step
(Protocols Name Carge Field (20 kVp) Medium Field (20 kVp) Medium Field, Sharp Filter(120 kVp) Small Pattert Large Field (200 kVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 12/17/2014 3:38 12/15/2014 4:23 12/17/2014 3:43 12/15/2014 4:28 12/19/2014 10:3(12/15/2014 4:34	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n Geo Place Centerir 5/2014 3:35 P 12/19/2014 11:39 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:25 P 12/19/2014 11:38 Ideal Rotation	ng Tor Click to start	:ol gain and offset
(Protocols Nam Large Field (120 kVp) Medium Field (120 kVp) Medium Field, Sharp Filter(120 kVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 2/17/2014 3:38 12/15/2014 4:28 2/17/2014 3:43 12/15/2014 4:28	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n Geo Place Centerir 5/2014 3:35 P 12/19/2014 11:39 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:25 P 12/19/2014 11:38 Ideal Rotation	In Center => 0	col gain and offset lone before this step
(Protocols Name Carge Field (20 kVp) Medium Field (20 kVp) Medium Field, Sharp Filter(120 kVp) Small Patient Large Field (200 kVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 12/17/2014 3:38 12/15/2014 4:23 12/17/2014 3:43 12/15/2014 4:28 12/19/2014 10:3(12/15/2014 4:34	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n Geo Place Centerir 5/2014 3:35 P 12/19/2014 11:39 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:25 P 12/19/2014 11:38 Ideal Rotation	In Center => 0 Lower Variance	col gain and offset lone before this step
(Protocols Name Carge Field (20 kVp) Medium Field (20 kVp) Medium Field, Sharp Filter(120 kVp) Small Patient Large Field (200 kVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 12/17/2014 3:38 12/15/2014 4:23 12/17/2014 3:43 12/15/2014 4:28 12/19/2014 10:3(12/15/2014 4:34	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n Geo Place Centerir 5/2014 3:35 P 12/19/2014 11:39 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:38 5/2014 3:28 P 12/19/2014 11:28	In Center => 0	col gain and offset lone before this step
(Protocols Name Carge Field (20 kVp) Medium Field (20 kVp) Medium Field, Sharp Filter(120 kVp) Small Patient Large Field (200 kVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 12/17/2014 3:38 12/15/2014 4:23 12/17/2014 3:43 12/15/2014 4:28 12/19/2014 10:3(12/15/2014 4:34	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n 6e0 5/2014 3:35 P 12/19/2014 11:38 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:26 P 12/19/2014 11:39 5/2014 3:28 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:28 S/2014 3:28 P 12/19/2014 11:28 S/2014 3:28 P 12/19/2014 11:28	In Center => 0 Lower Variance	sol gain and offset Jone before this step Is Centering Acceptable? First Center
(Protocols Name Carge Field (20 kVp) Medium Field (20 kVp) Medium Field, Sharp Filter(120 kVp) Small Patient Large Field (200 kVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 12/17/2014 3:38 12/15/2014 4:23 12/17/2014 3:43 12/15/2014 4:28 12/19/2014 10:3(12/15/2014 4:34	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n 6e0 5/2014 3:35 P 12/19/2014 11:38 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:26 P 12/19/2014 11:39 5/2014 3:28 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:28 S/2014 3:28 P 12/19/2014 11:28 S/2014 3:28 P 12/19/2014 11:28	In Center => 0 Lower Variance	:01 gain and offset lone before this step Is Centering Acceptable?
(Protocols Narr Large Field (120 KVp) Medium Field (120 KVp) Medium Field (120 KVp) Small Patient: Large Field (100 KVp) Small Patient: Medium Field (100 KVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 12/17/2014 3:38 12/15/2014 4:23 12/17/2014 3:43 12/15/2014 4:28 12/19/2014 10:3(12/15/2014 4:34	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n Geo Place Centerir 5/2014 3:35 P 12/19/2014 11:39 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:23 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:38 5/2014 3:28 P 12/19/2014 11:28	In Center => 0 Lower Variance	sol gain and offset Jone before this step Is Centering Acceptable? First Center
(Protocols Narr Large Field (120 KVp) Medium Field (120 KVp) Medium Field (120 KVp) Small Patient: Large Field (100 KVp) Small Patient: Medium Field (100 KVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 2/17/2014 3:28 12/15/2014 4:42 12/15/2014 10:81 12/15/2014 4:38 12/15/2014 10:81 12/15/2014 4:38 12/15/2014 4:12	Gain Cal Norr 12/15/2014 3d5 P 12/15 12/15/2014 3d5 P 12/15	n 5/2014 3:35 P 12/19/2014 11:39 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:28 10.00000000000000000000000000000000000	In Center => 0 Lower Variance	sol gain and offset Jone before this step Is Centering Acceptable? First Center
	Protocols Narr Large Field (120 KVp) Medium Field (120 KVp) Medium Field (120 KVp) Small Patient: Large Field (100 KVp) Small Patient: Medium Field (100 KVp)	LP Water 12/17/2014 3:26 12/15/2014 4:47 12/17/2014 3:38 12/15/2014 4:23 12/17/2014 3:43 12/15/2014 4:28 12/19/2014 10:3(12/15/2014 4:34	Gain Cal Norm 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15 12/15/2014 3:15 P 12/15	n 6e0 5/2014 3:35 P 12/19/2014 11:38 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:25 P 12/19/2014 11:28 5/2014 3:26 P 12/19/2014 11:39 5/2014 3:28 P 12/19/2014 11:28 5/2014 3:28 P 12/19/2014 11:28 S/2014 3:28 P 12/19/2014 11:28 S/2014 3:28 P 12/19/2014 11:28	In Center => 0 Lower Variance	sol gain and offset Jone before this step Is Centering Acceptable? First Center

Click on the Find Center of rotation tab and the following will appear:

Select the Medium Field (120 kVp) protocol from the list, it will be highlighted blue when selected. Click on the Find Center OK button and instructions will appear that will include instructions to fire the x-ray. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

During the calibrations, the screen will turn light gray and an image will appear in the window at the top as shown below:

B Sde		Ref Bio 3.5X Unsigned 16-bit image 43600 (0)	A Side	
AVB/Center Distance Measurement General System Information Inn Protocols Name Large Field (120 KVp) Medium Field (120 KVp) Small Patient: Large Field (100 KVp) Small Patient: Medium Field (100 KVp)	Advanced Quality Tess ge Quality Analysis Panel Gain Calibratis Jeen 12/17/2014 326 12/15/2014-447 12/15/2014 12/17/2014 326 12/15/2014 428 12/15/2014 12/17/2014 326 12/15/2014 428 12/15/2014 12/19/2014 10-81 12/15/2014 428 12/15/2014 12/15/2014 421 12/15/2014 428 12/15/2014	Normalization File Creation for Reco 15 P 12/15/2014 33.5 P 12/19/2014 11.30 35 P 12/15/2014 33.2 P 12/19/2014 11.20 35 P 12/15/2014 33.2 P 12/19/2014 11.20 35 P 12/15/2014 33.2 P 12/19/2014 11.20 35 P 12/15/2014 33.2 P 12/19/2014 11.20	Reconstruction Leg DataBase Single Sho naturation engine Geometric Analysis and File Creation Place Centering Tool in Scanner - Select a Mediu Upper Variance 0 0 Ideal Rotation Center Nearuret Rotation Center 383.5 0 Lower Variance 0	Find Center of rotation IN FOV Protocol Note: crude gain and offset need to be done before this step
Room Door Ready	Xray Service Fault	Complete Busy	Procedure Run	EXIT

Once the calibration is completed the "Is Centering Acceptable" light will either be red or green. The below shows a successful calibration:

B Side	Center		A Side
	1536x1536	5 0.18X Float image 9000.00 (0	
12			indicates
A/B/Center Distance Measurement General System Information	Advanced Quality Tests Collimator Setup age Quality Analysis Panel Gain Calibration	View Cal Files Firmward Normalization File Creation f SUCCES	Single Shot Motor, LED, Xray Control
General system anomation and	age Quality Analysis		s, reu
Protocols		failure	
Name		orm Geo	elect a Medium FOV Protocol
Large Field (120 kVp) Medium Field (120 kVp)	12/17/2014 3:26 12/15/2014 4:47 12/15/2014 3:15 P 12 12/17/2014 3:38 12/15/2014 4:23 12/15/2014 3:15 P 12		Upper Variance Noter sure gain and offset
Medium Field, Sharp Filter(120 kVp)	12/17/2014 3:43 12/15/2014 4:28 12/15/2014 3:15 P 12	2/15/2014 3:23 P 12/19/2014 11:28	50.5822 ced to be done before the step
Small Patient: Large Field (100 kVp)	12/19/2014 10:36 12/15/2014 4:34 12/15/2014 3:15 P 12	2/15/2014 3:26 P 12/19/2014 11:39 Ideal Ro	otation Center Measured Rotation Center Is Centering Acceptable?
Small Patient: Medium Field (100 kVp)	12/15/2014 4:12 12/15/2014 4:38 12/15/2014 3:15 P 12	2/15/2014 3:28 P 12/19/2014 11:28 383.5	=> 383.605
			Lower Variance
			15.3427 Find Center
<			OK
Room Door Ready	Xray Service Fault	Complete Busy	
			EXIT

If the centering is not successful, and the Is Centering Acceptable light is red, then perform the A/B/Center Distance Measurement and come back and rerun this Find Center of Rotation calibration a second time. If after performing these calibrations it is still unsuccessful, please contact Technical Support.

A/B/Center Distance Measurement

Leave the Centering Tool from the last calibration in the scanner for this calibration as well.

Click on the A/B/Center Distance Measurement tab and the following will be displayed:

	B Side	Center A Side
Q		
	General System Information Image Quality Analysis Panel Gain Calibr	ation Normalization File Creation for Reconstruction engine
	A/B/Center Distance Measurement Advanced Quality Tests Collimators	
	BPoints C - 8 (horiz / vert) 0.00 0.00 0.00 0.00 0.00 0.00	Center Points A -C (horiz / vert) Onton Dob Dob <thd< th=""></thd<>
	Position in Degrees Slope B / C / A	A - 8 (horiz / vert) rotation 0.00 0.00 (ideal=0) 0.00 0.00 0.00 0.00 0.00 0.00 0.00 - 1565 OK
	DataBase Values -> 1919656 ACtr Distance DataBase Values -> 1919656 ACtr Distance Centering kVp 980778 Ctr-8 Distance 120 panel_offset_to_b 940208	Ashould be Ashould be Ashould be Actr Dist appear here Actr Dist appear here
	Room Door Ready Xray Service Fault	Complete Busy OpenDoors(AfterScan)


Click on the Get Align Images / Compute Values OK button and instructions will appear that will include instructions to fire the x-ray. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure


During the calibration, the screen will go light gray and images will appear in the top windows, similar those below:

8 Side		Center	ASde	(556,665)
		^Should be ^Should be 1200 = 0 191963		
	ffset_to_b 940208		anel_off_to_b 0 Reset To Defaults OK	
Room Door Ready	Xray Service Fau	lt Complete Busy	Press and HOLD Scan button	


Once the calibration is completed, the results will need to be checked. The ideal rotation is 0 +/-1.0 and can be found in the center of the screen. If an adjustment is needed, it is shown below the ideal rotation value in terms of turns needed, where ccw means counter clockwise.

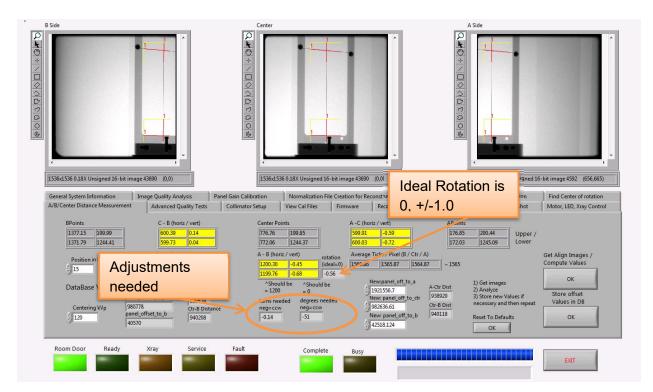

The values of concern, in a larger picture are as shown below:




The adjustments are shown both in turns needed and degrees. Use the format that is most comfortable. If adjustments are needed, adjust the screws on the mounting plate for the panel as shown below:

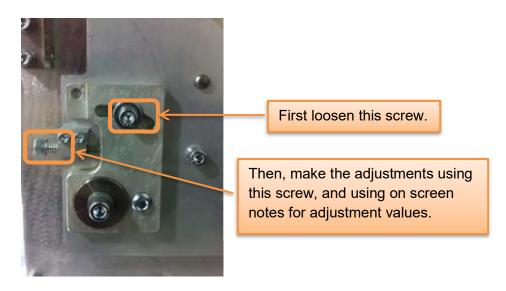

If the adjustments are needed, once made, rerun this calibration.

If the values are in the good range, 0 +/- 1.0, then this calibration is successful and the values should be stored, click the OK for "Store offset values in DB".

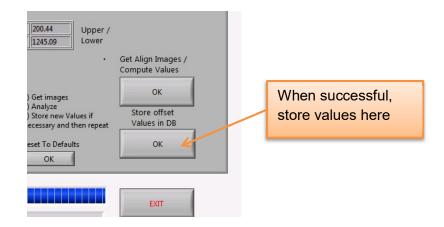

Advanced Quality Tests – Line Pairs and Water

Remove the Centering Tool from the scanner. Place the Patient Platform back into position in the scanner too.

Place the QA Phantom (Line Pair Phantom) in the scanner. This should be centered using the patient positioning circle on the Patient Platform.

Click on the Advanced Quality Tests tab.

	B Side				Center					A Side		
3171001+13 *0			ŕ					Î				
003		LP Colum	n is po	nulate	d				0			
0			-	pulate	u l				0			
_		with succe	esstul							1		
	•	calibration	ns/tests	S				w. F		•		• •
Í												[
1	General Sys	tem Information Ima	ge Quality Analys	e Panel (Gain Calibration	Normalization File	Creation for Recons	truction engine	Geometric	Analysis and	File Creation	Find Center of rotation
		Distance Measurement	Advar ced Quali		ollimator Setup	View Cal Files	× 1	econstruction	N. N.	lataBase	Single Shot	Motor, LED, Xray Control
	Protocols									ce	Correct Test Pi	antom in Scanner
	Name	(LP	Water	Gain Cal	Norm Geo	Click (OK to s	start	:e9		Wsize% Wstart%
		ld (120 kVp) Field (120 kVp)	12/17/2014 3:26 needed			P 12/15/2014 3:35 P 12/ P 12/15/2014 3:21 P 12/	OA/I in	ne Pair	· test		0.04	0.01 0.5
		Field, Sharp Filter(120 kVp) ient: Large Field (100 kVp)				P 12/15/2014 3:23 P 12/ P 12/15/2014 3:26 P 12/			1031	.PP	hantom	Scan WaterPhantom
		ient: Medium Field (100 kVp)				P 12/15/2014 3:28 P 12/		_			ок.	ОК
	-							ReconStart		Analyze I	LPPhantom	Analyze WaterPhantom
	-					1 1	<u> </u>	-		Ť	ок	ОК
	لشر											
,	Room D	oor Ready	Xray	Service	Fault	Complete	Busy	1			-	
	-					complete	Busy					EXIT


For this calibration, each protocol will need to be run for the QA Phantom. As each calibration is completed, the date will be placed in the LP column above. Highlight the first protocol and click OK under the Anaylze LPPhantom. This will start the calibration and instructions will appear that will include instructions to fire the x-ray. When prompted, Press and Hold the Scan button to fire the x-ray.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

During the calibration, the screen will go light gray and images will appear in the top windows, similar those below:

B Side	Center	0.36X Unsigned 16-bit image 43690 (0,0)		A Side	
General System Information In A/B/Center Distance Measurement Protocols	age Quality Analysis Panel Gain Calibration Advanced Quality Tests Collimator Setup			Analysis and File Creation taBase Single Shot	Find Center of rotation Motor, LED, Xray Control antom in Scanner
Name Large Field (120 kVp) Medium Field (120 kVp)	12/17/2014 3:26 12/15/2014 4:47 12/15/2014 3:15 P 1 needed 12/15/2014 4:23 12/15/2014 3:15 P 1	Norm Geo A 12/15/2014 3:35 P 12/19/2014 11:39 12/15/2014 3:21 P 12/19/2014 11:28		LPsize% LPstart%	
Medium Field, Sharp Filter(120 kVp) Small Patient: Large Field (100 kVp) Small Patient: Medium Field (100 kVp)	12/17/2014 3:43 12/15/2014 4:28 12/15/2014 3:15 P 12/19/2014 10:36 12/15/2014 4:34 12/15/2014 3:15 P 1 12/15/2014 4:12 12/15/2014 4:38 12/15/2014 3:15 P	12/15/2014 3:26 P 12/19/2014 11:39	ReconDone	OK	ОК
					Analyze WaterPhantom
		<u>x</u>		ΟΚ	ОК
Room Door Ready	Xray Service Fault	Complete Busy	Procedure Run		EXIT

Once completed, the results screen will appear similar to below:

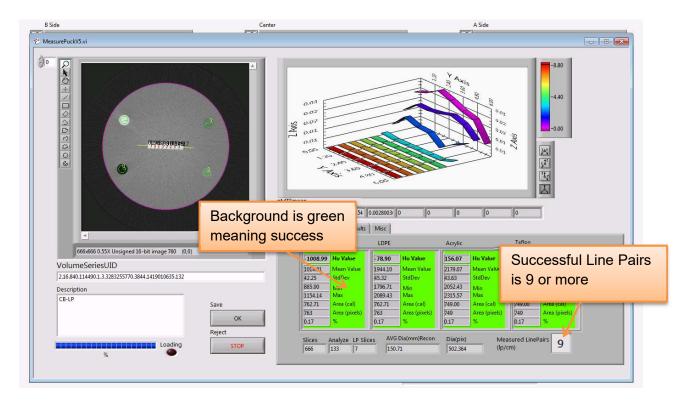

To determine if it was a success, observe the colors behind the numbers – if they are all green, and the Measured LinePairs is 9 or above, this is successful and the Save OK

button should be selected. If the backgrounds are not green or the Measured LinePairs is 8 or less, then Reject this scan, click the STOP under the Reject and contact Technical Support.

Perform this test on all of the Protocols.

Once all of the protocols have been successfully completed for the QA Phantom, remove the QA Phantom from the field of view. Place the Water Phantom in the field of view.

Next perform the water calibration, still on the same tab, for each of the protocols. This is done very similar to the QA Phantom (Line Pairs) testing, the only exception being that the Analyze WaterPhantom OK button is selected to start the entire process.

	Water Colu populated v calibrations	vith successf	ul		A Side	
A/B/Center Distance Measurement	ge Quality Analysis Par Advanced Quality Tests	H Gain Calibration Norm Collimator Setup View C	alization File Creation for Reco al Files Firmware	Reconstruction Log	cometric Analysis and File Creation DataBase Single Shot Description Place Correct	Find Center of rotation Motor, LED, Xray Control
Protocols Name Large Field (120 kVp) Medium Field (120 kVp) Small Patient: Large Field (100 kVp) Small Patient: Medium Field (100 kVp)	needed 12/15/2014 4 12/17/2014 3:43 12/15/2014 4 12/19/2014 10:36 12/15/2014 4	Gain Cal Norm 147 12/15/2014 3:15 P 12/15/201 122 12/15/2014 3:15 P 12/15/201 123 12/15/2014 3:15 P 12/15/201 124 12/15/2014 3:15 P 12/15/201 124 12/15/2014 3:15 P 12/15/201 134 12/15/2014 3:15 P 12/15/201 138 12/15/2014 3:15 P 12/15/201	4 3:21 P 12/19/2014 11:28 4 3:23 P 12/19/2014 11:28 4 3:26 P 12/19/2014 11:39	Store this Series with D	LPsize% LPst C	lick OK to start /ater Phantom tests
	Xray Service	Fault	Complete Busy	[]		EXIT

Perform the Analyze WaterPhantom test on each of the protocols. As each calibration is completed, the date will be placed in the Water column above.


Perform this test on all of the Protocols.

Once all of the protocols have been successfully completed for the QA Phantom, remove the Water Phantom from the field of view.

Collimator Setup

Ensure that all items are removed from the field of view, including the Patient Platform.


Click on the Collimator Setup Tab. The following should appear:

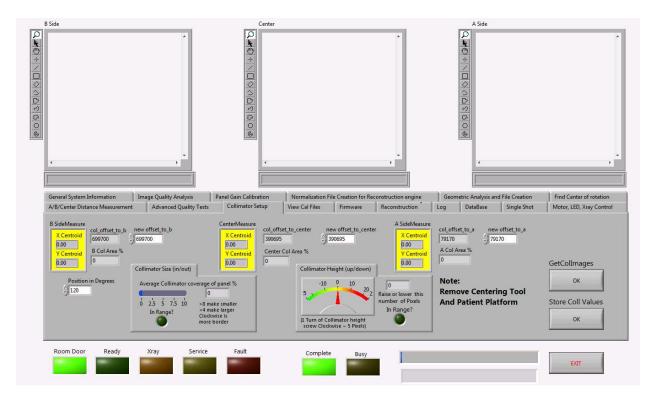

Click on the GetCollmages OK button to start the calibration. This will start the calibration and instructions will appear that will include instructions to fire the x-ray. When prompted, Press and Hold the Scan button to fire the x-ray. X-ray will be fired **THREE** times.

WARNING The X-ray device may be dangerous to the Patient and Operator if you do not observe and follow operating instructions. Do not operate this system unless you have received training to perform a procedure

As the x-ray fires each of the three times, one of the windows above will have an image, and the screen will become a light gray. After all three shots have been fired, the following will appear:

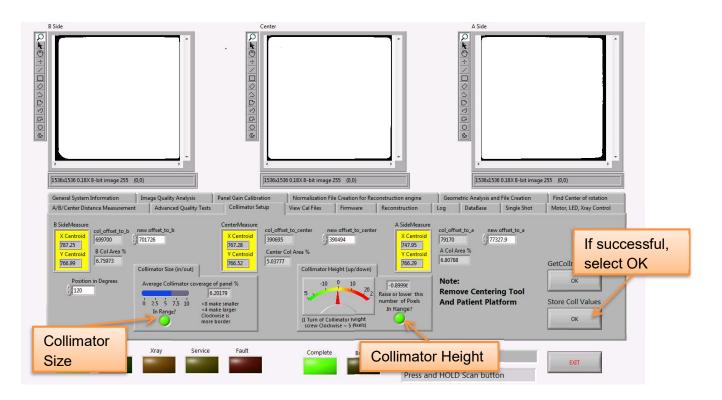


Successful completion is two green lights, one in the Collimator Size and one in the Collimator Height boxes. If both lights are green, select the StoreColValues OK button.

If the lights are not green, a mechanical adjustment is needed.

If the Collimator Size is not green it needs to be adjusted. The acceptable Collimator Size (in/out) range is between 4-8%. Instructions on screen are given for adjustments. Turning the higher screw clockwise will provide more border around the images by moving away from the tube head and closer to the panel.

If the Collimator Height is not green it needs to be adjusted. The acceptable Collimator Height (up/down) range is 0 +/- 5 pixels. Instructions on screen are given for adjustments. Turning the lower screw clockwise will cause it to move up.

If adjustments are needed, it may be necessary to manually rotate the gantry to get to the Collimator Adjustment Screws. Below is an image of the collimator adjustment screws, depicting which screw to use for each adjustment needed to the collimator:

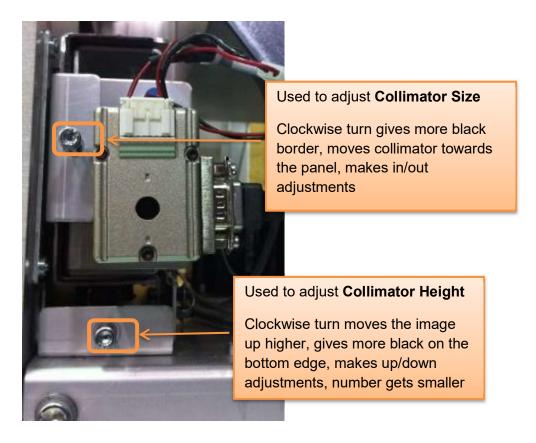

If any adjustments are needed, the present values must be stored first before the calibration is continued. Select Store Coll Values OK button in the lower right corner to store the current values. Then restart this calibration by clicking GetCollmages OK again. Revisit the images and values as mentioned above. Repeat these steps until the images appear as shown above and the values are as presented above.

Once the two buttons are green (one for height, one for size), select Store Coll Values OK in the lower right corner to store the current values for this calibration.

Place the Patient Platform in the scanner.

All calibrations are complete.